

SECULIFE DF+

DEFIBRILLATOR ANALYZER

3-349-622-03
1/3.11



Contents

WARNINGS, CAUTIONS, NOTICES.....	5
DESCRIPTION	11
OVERVIEW.....	19
DEFIBRILLATOR ANALYZER.....	26
MAIN SCREEN	26
ECG WAVEFORMS SCREEN.....	33
PLAYBACK LAST PULSE SCREEN	37
START CHARGE TIMER SCREEN.....	39
PRINT HEADER	41
SELF TEST WAVEFORM.....	43
RUNNING A DEFIBRILLATION TEST	45
INTRODUCTION.....	45
DEFIBRILLATION TEST	47
CARDIOVERSION TEST	50
CHARGE TIME TEST	55
SHOCK ADVISORY ALGORITHM TEST	57
TRANSCUTANEOUS PACEMAKER ANALYZER.....	59
PACE MAIN SCREEN	59
PACER MODE SETUP SCREEN.....	65
SENSITIVITY TEST	67
REFRACTORY PERIOD TEST	69
PRINT MENU SCREEN.....	71
PLAYBACK LAST PULSE SCREEN	73

MESSAGES	75
SYSTEM SETUP	77
POWER UP SETTINGS.....	79
AUTO SEQUENCE FUNCTION.....	81
VIEW MODE	83
RUN MODE.....	87
PROGRAMMING AUTOSEQUENCES.....	97
WARRANTY.....	109
SPECIFICATIONS	110

WARNING - USERS

The SECULIFE DF+ analyzer is for use by skilled technical personnel only.

WARNING - USE

The SECULIFE DF+ Analyzer is intended for testing only and it should never be used in diagnostics, treatment or any other capacity where it would come in contact with a patient.

WARNING - MODIFICATIONS

The SECULIFE DF+ Analyzer is intended for use within the published specifications. Any application beyond these specifications or any unauthorized user modifications may result in hazards or improper operation.

WARNING - CONNECTIONS

All connections to patients must be removed before connecting the Device Under Test (DUT) to the Analyzer. A serious hazard may occur if the patient is connected when testing with the Analyzer.

Do not connect any leads from the patient directly to the Analyzer or DUT.

WARNING - POWER ADAPTER

Unplug the Power Adapter before cleaning the surface of the Analyzer.

WARNING - LIQUIDS

Do not submerge or spill liquids on the Analyzer. Do not operate the Analyzer if internal components not intended for use with fluids may have been exposed to fluid, as the internal leakage may have caused corrosion and be a potential hazard.

CAUTION - SERVICE

The SECULIFE DF+ Analyzer is intended to be serviced only by authorized service personnel. Troubleshooting and service procedures should only be performed by qualified technical personnel.

CAUTION - ENVIRONMENT

The SECULIFE DF+ Analyzer is intended to function between 15 and 40 °C. Exposure to temperatures outside this range can adversely affect the performance of the Analyzer.

CAUTION - CLEANING







Do not immerse. The Analyzer should be cleaned by wiping gently with a damp, lint-free cloth. A mild detergent can be used if desired.

CAUTION - INSPECTION

The SECULIFE DF+ Analyzer should be inspected before each use for wear and the Analyzer should be serviced if any parts are in question.

NOTICE – INDICATIONS FOR USE

The SECULIFE DF+ Analyzer is used to determine that defibrillators and transcutaneous pacemakers are performing within their performance specifications through the measurement of energy output.

NOTICE – SYMBOLS <u>Symbol</u>	<u>Description</u>
	Caution (Consult Manual for Further Information)
	Hazardous Voltage
	Center Negative
	Direct Current
	Per European Council Directive 2002/95/EC, do not dispose of this product as unsorted municipal waste.
	Conforms to European Union directives
CAT I	IEC Measurement Category I – CAT I equipment designed to protect against transients in equipment on circuits not directly connected to MAINS. Under no circumstances should the terminals of the Analyzer be connected to any MAINS voltage

NOTICE – ABBREVIATIONS

A, Amps	Amperes
BPM	Beats Per Minute
c	centi- (10^{-2})
C	Celsius
°	degree
dt	Delta Time, Change in Time
DUT	Device Under Test
E	Energy
ECG	Electrocardiogram
Euro	European
Hz	hertz³)
kg	kilograms
lbs	pounds
μ	micro- (10^{-6})
μA	microampere
μH	microhertz
μV	microvolt
μsec	microsecond
m	milli- (10^{-3})-
mA	milliampere
mm	millimeter
ms, mS, msec	millisecond
mV	millivolts
Ω	ohm
P	Power
ppm	pulse per minute
R	Resistance, ohms
Sec, S	seconds
US	United States
V	volt
VDC	Direct Current Voltage



EG - KONFORMITÄTSERKLÄRUNG
DECLARATION OF CONFORMITY

GMC-I  MESSTECHNIK

Dokument-Nr./ Document.No.: 820 / 11-016
 Hersteller/ Manufacturer: GMC-I GOSSEN-METRAWATT GMBH
 Anschrift / Address: Südwestpark 15
 D - 90449 Nürnberg
 Produktbezeichnung/ Product name: Defibrillator Analyser
 Defibrillator Analyser
 Typ / Type: SECULIFE DF+
 Bestell-Nr / Order No: M695A

Das bezeichnete Produkt stimmt mit den Vorschriften folgender Europäischer Richtlinien überein, nachgewiesen durch die vollständige Einhaltung folgender Normen:

The above mentioned product has been manufactured according to the regulations of the following European directives proven through complete compliance with the following standards:

Nr. / No.	Richtlinie	Directive
2006/95/EG 2006/95/EC	Elektrische Betriebsmittel zur Verwendung innerhalb bestimmter Spannungsgrenzen - Niederspannungsrichtlinie – Anbringung der CE-Kennzeichnung : 2011	Electrical equipment for use within certain voltage limits - Low Voltage Directive - Attachment of CE mark : 2011

<u>EN/Norm/Standard</u>	<u>IEC/Deutsche Norm</u>	<u>VDE-Klassifikation/Classification</u>
EN 61010-1 : 2001	IEC 61010-1 : 2001	VDE 0411-1 : 2002


Nr. / No.	Richtlinie	Directive
2004/108/EG 2004/108/EC	Elektromagnetische Verträglichkeit - EMV Richtlinie -	Electromagnetic compatibility - EMC directive -

Fachgrundnorm / Generic Standard

EN 61326-1 : 2006

Nürnberg, den 10.02.2011

Ort, Datum / Place, date:


Geschäftsführung / managing director

Diese Erklärung bescheinigt die Übereinstimmung mit den genannten Richtlinien, beinhaltet jedoch keine Zusicherung von Eigenschaften. Die Sicherheitshinweise der mitgelieferten Produktdokumentationen sind zu beachten.

This declaration certifies compliance with the above mentioned directives but does not include a property assurance. The safety notes given in the product documentations, which are part of the supply, must be observed.

NOTICE – DISCLAIMER

USER ASSUMES FULL RESPONSIBILITY FOR UNAUTHORIZED EQUIPMENT MODIFICATIONS OR APPLICATION OF EQUIPMENT OUTSIDE OF THE PUBLISHED INTENDED USE AND SPECIFICATIONS. SUCH MODIFICATIONS OR APPLICATIONS MAY RESULT IN EQUIPMENT DAMAGE OR PERSONAL INJURY.

NOTICE – DISCLAIMER

GMC-I MESSTECHNIK GMBH RESERVES THE RIGHT TO MAKE CHANGES TO ITS PRODUCTS OR SPECIFICATIONS AT ANY TIME, WITHOUT NOTICE, IN ORDER TO IMPROVE THE DESIGN OR PERFORMANCE AND TO SUPPLY THE BEST POSSIBLE PRODUCT. THE INFORMATION IN THIS MANUAL HAS BEEN CAREFULLY CHECKED AND IS BELIEVED TO BE ACCURATE. HOWEVER, NO RESPONSIBILITY IS ASSUMED FOR INACCURACIES.

NOTICE – CONTACT INFORMATION

**GMC-I Messtechnik GmbH
Südwestpark 15
90449 Nürnberg
Germany
Phone: +49 911 8602-111
Fax: +49 911 8602-777**

**www.gossenmetrawatt.com
[e-mail: info@gossenmetrawatt.com](mailto:info@gossenmetrawatt.com)**

DEFIBRILLATOR ANALYZER

SECULIFE DF+ is a microprocessor-based instrument that is used in the testing of defibrillators. It measures the energy output and provides information about the defibrillation pulse. It is used on manual, semi-automatic and automatic defibrillators with monophasic or biphasic outputs.

SECULIFE DF+ additionally provides a Transcutaneous Pacemaker analysis function. It measures and displays pacer pulse information as well as performing Refractory Period, Sensitivity and Immunity testing.

It has a built in 50 ohm human body simulation load as well as 12 lead ECG with arrhythmias and performance waveforms. Additionally, it has a Centronics printer port, a serial port, oscilloscope output, high-level ECG output, as well as provision for a battery eliminator.

SECULIFE DF+ makes viewing and selecting the desired waveforms and test data quick and intuitive, with all operational information being available on the 240 by 64 pixel graphic display, allowing for easy maneuvering through parameters and scrolling through available options.

NOTE

**This instrument is intended for use by
Trained Service Technicians.**

The following are highlights of some of the main features:

GENERAL

- SIMPLE TO OPERATE
- GRAPHICS DISPLAY WITH SIMULTANEOUS DETAILED STATUS OF PARAMETERS AND SCROLLING CONTROL OF OPTIONS
- ON SCREEN VIEWING OF DEFIBRILLATOR AND PACEMAKER WAVEFORMS
- DROP DOWN CHOICE SCREENS LIST ALL OPTIONS FOR PARAMETERS
- MONOPHASIC AND BIPHASIC COMPATIBLE
- 5000 V, 1000 JOULE CAPACITY
- HIGH AND LOW RANGES
- CARDIOVERSION DELAY MEASUREMENT
- CHARGE TIME MEASUREMENT
- WAVEFORM STORAGE AND PLAYBACK
- 10 UNIVERSAL PATIENT LEAD CONNECTORS
- 25 PIN CONNECTOR FOR CENTRONICS PRINTER
- 9 VOLT BATTERY POWER
- LOW BATTERY INDICATOR
- AVAILABLE BATTERY ELIMINATOR
- DISPLAY BACKLIGHT
- FULL REMOTE OPERATION VIA RS-232
- FLASH PROGRAMMABLE FOR UPGRADES
- AUTO SEQUENCE TESTING CAPABLE OF STORING 50 CUSTOM TEST SEQUENCES

PACEMAKER FUNCTION

- 26 SELECTABLE INTERNAL LOADS
- FULL PULSE ANALYSIS
- DEMAND SENSITIVITY TEST
- REFRACTORY PERIOD TESTS
- 50/60 Hz INTERFERENCE TEST SIGNALS
- INPUT TERMINALS AND CIRCUITRY PROTECTED AGAINST ACCIDENTAL DEFIBRILLATOR DISCHARGE INTO PACEMAKER TEST TERMINALS

ENERGY OUTPUT MEASUREMENT GENERAL

The unit measures the energy in the output pulse of both monophasic and biphasic defibrillators.

- PULSE TYPE: Monophasic or Biphasic
- LOAD RESISTANCE: 50 ohm +/- 1%, non-inductive (<1 μ H)
- DISPLAY RESOLUTION: 0.1 Joules
- MEASUREMENT TIME WINDOW: 100 ms
- ABSOLUTE MAX PEAK VOLTAGE: 6000 Volts
- CARDIOVERSION DELAY: 0 to 6000 ms
- CARDIOVERSION RESOLUTION: 0.1 ms

ENERGY OUTPUT MEASUREMENT HIGH RANGE

The high range allows for a large pulse with high voltage and current.

- VOLTAGE: \leq 5000 Volts
- MAX CURRENT: 100 Amps
- MAX ENERGY: 1000 Joules
- TRIGGER LEVEL: 100 Volts
- PLAYBACK AMPLITUDE: 1 mV / 1000 V Lead I
- TEST PULSE: 125 Joules +/- 20%

ENERGY OUTPUT MEASUREMENT LOW RANGE

The low range allows greater resolution on smaller pulses.

- VOLTAGE: <1000 Volts
- MAX CURRENT: 20 Amps
- MAX ENERGY: 50 Joules
- TRIGGER LEVEL: 20 Volts
- PLAYBACK AMPLITUDE: 1 mV / 1000 V Lead I
- TEST PULSE: 5 Joules +/- 20%

ENERGY OUTPUT MEASUREMENT OTHER

OSCILLOSCOPE OUTPUT

- HIGH MEASUREMENT RANGE: 1000:1 amplitude-attenuated
- LOW MEASUREMENT RANGE: 200:1 amplitude-attenuated

WAVEFORM PLAYBACK

- OUTPUT – LEAD 1 & PLATES
- GRAPHICS SCREEN
- 200:1 Time Base Expansion

SYNC TIME MEASUREMENTS

- TIMING WINDOW: Starts at peak of each R-wave
- TEST WAVEFORMS: All waveform simulations available

CHARGE TIME MEASUREMENT

- From 0.1 to 99.9 sec

ECG FUNCTIONS

The unit can produce a wide variety of ECG simulations. The user simply selects the parameters that match the desired output.

- RATE: 30,40,45,60,80,90,100,120,140,160,180,200,220,240,260,280,300 BPM
- AMPLITUDE: 0.50,1.0,1.5,2.0 mV (Lead II)

ECG-PERFORMANCE FUNCTIONS

The unit can generate Sine, Square, Triangular, and Pulse waveforms with adjustable amplitudes for performance testing.

- SINE: 0.1,0.2,0.5,5,10,40,50,60,100 Hz
- SQUARE: 0.125,2 Hz
- TRIANGLE: 2,2.5 Hz
- PULSE: 30,60,120 BPM; 60 ms WIDTH
- AMPLITUDE: 0.5,1.0,1.5,2.0 mV (Lead II)

ARRHYTHMIA FUNCTIONS

The unit can simulate 12 different arrhythmias.

- VENTRICULAR FIBRILLATION
- ATRIAL FIBRILLATION
- SECOND DEGREE A-V BLOCK
- RIGHT BUNDLE BRANCH BLOCK
- PREMATURE ATRIAL CONTRACTION
- EARLY PVC
- STANDARD PVC
- R ON T PVC
- MULTIFOCAL PVC
- BIGEMINY
- RUN OF 5 PVC
- VENTRICULAR TACHYCARDIA

SHOCK ADVISORY TESTS

The unit can simulate 8 different waveforms to test the shock algorithm of advanced defibrillators:

- ASYSTOLE
- COARSE VENTRICULAR FIBRILLATION
- FINE VENTRICULAR FIBRILLATION
- MULTIFOCAL VENTRICULAR TACHYCARDIA @ 140 BPM
- MULTIFOCAL VENTRICULAR TACHYCARDIA @ 160 BPM
- POLYFOCAL VENTRICULAR TACHYCARDIA @ 140 BPM
- POLYFOCAL VENTRICULAR TACHYCARDIA @ 160 BPM
- SUPRAVENTRICULAR TACHYCARDIA @ 90 BPM

TRANSCUTANEOUS PACER ANALYZER

The unit can test external transcutaneous pacemakers. It has a wide variety of loads and can measure the Pacer Pulse, Demand Sensitivity and Refractory Periods (Pacing and Sensing):

- LOAD:
 - RANGE: 50,100,150,200,300,400,500,600,700,800,900,1000,1100,1200,1300,1400,1500,1600,1700,1800,1900,2000,2100,2200,2300 ohm
- PULSE:
 - PULSE CURRENT: 4 TO 300 mA (100 ohm load)
 - RATE: 30 TO 800 ppm
 - WIDTH: 0.6 to 80 ms
- DEMAND SENSITIVITY:
 - WAVEFORMS:
 - SELECTIONS: SQUARE, TRIANGLE, HAVERSINE
 - WIDTH: 10,25,40,100,200 ms
 - ECG:
 - AMPLITUDE – OUT: 0 to 4 mV
 - PACER INPUT (50 TO 400 OHM):
 - AMPLITUDE – OUT: 0 to 10 mV / 50 ohms
 - RATE – IN: 30 to 100 ppm
 - PACER INPUT (500 TO 2300 OHM & OPEN):
 - AMPLITUDE – OUT: 0 to 100 mV
 - RATE – IN: 30 to 100 ppm
 - DEFIBRILLATOR PLATES:
 - AMPLITUDE – OUT: 0 to 10 mV
 - RATE – IN: 30 to 100 ppm
- REFRACTORY PERIOD:
 - PACING: 20 to 500 ms
 - SENSING: 20 to 500 ms
- 50/60 HZ INTERFERENCE TEST SIGNAL:
 - ECG OUTPUT: 0,0.4,0.8,1.2,1.6,2.0,2.4,2.8,3.2,3.6,4.0 mV
 - PACER INPUT 50 OHM: 0,1,2,3,4,5,6,7,8,9,10 mV
 - PACER INPUT 100 OHM: 0,2,4,6,8,10,12,14,16,18,20 mV
 - PACER INPUT 150 OHM: 0,3,6,9,12,15,18,21,24,27,30 mV
 - PACER INPUT 200 OHM: 0,4,8,12,16,20,24,28,32,26,40 mV
 - PACER INPUT 300 OHM: 0,6,12,18,24,30,36,42,48,54,60 mV
 - PACER INPUT 400 OHM: 0,8,16,24,32,40,48,56,64,72,80 mV
 - PACER INPUT \geq 500 OHM: 0,10,20,30,40,50,60,70,80,90,100 mV
 - DEFIBRILLATOR PLATES: 0,1,2,3,4,5,6,7,8,9,10 mV
- INPUT CIRCUITRY PROTECTION
 - INPUT CIRCUITRY IS PROTECTED AGAINST DAMAGE IN THE EVENT OF AN ACCIDENTAL DEFIBRILLATOR DISCHARGE INTO THE PACEMAKER TEST INPUT TERMINALS

ACCESSORIES

BC20 - 40032	INTERNAL PADDLE ADAPTERS (2 adapters)
BC20 - 21103	BATTERY ELIMINATOR (120 VAC) (US Version)
BC20 - 21101	BATTERY ELIMINATOR (220 VAC) (Euro Version)
BC20 - 00427	PLASTIC ELECTRODE PLATES (2 plates)


OPTIONAL ACCESSORIES

BC20 - 30108	MEDIUM SOFT SIDED CARRYING CASE
BC20 - 41341	COMMUNICATION CABLE (DB 9 M to DB 9 F)
BC20 - 00420	PHYSIO-CONTROL DEFIB / PACE TEST CABLE
BC20 - 00421	MARQUETTE DEFIB / PACE TEST CABLE
BC20 - 00423	ZOLL DEFIB/PACE TEST CABLE
BC20 - 00426	HP / AGILENT / LAERDAL / AAMIDEFIB / PACE TEST CABLE


This page intentionally left blank.

OVERVIEW

This section looks at the layout of SECULIFE DF+ and gives descriptions of the elements that are present.

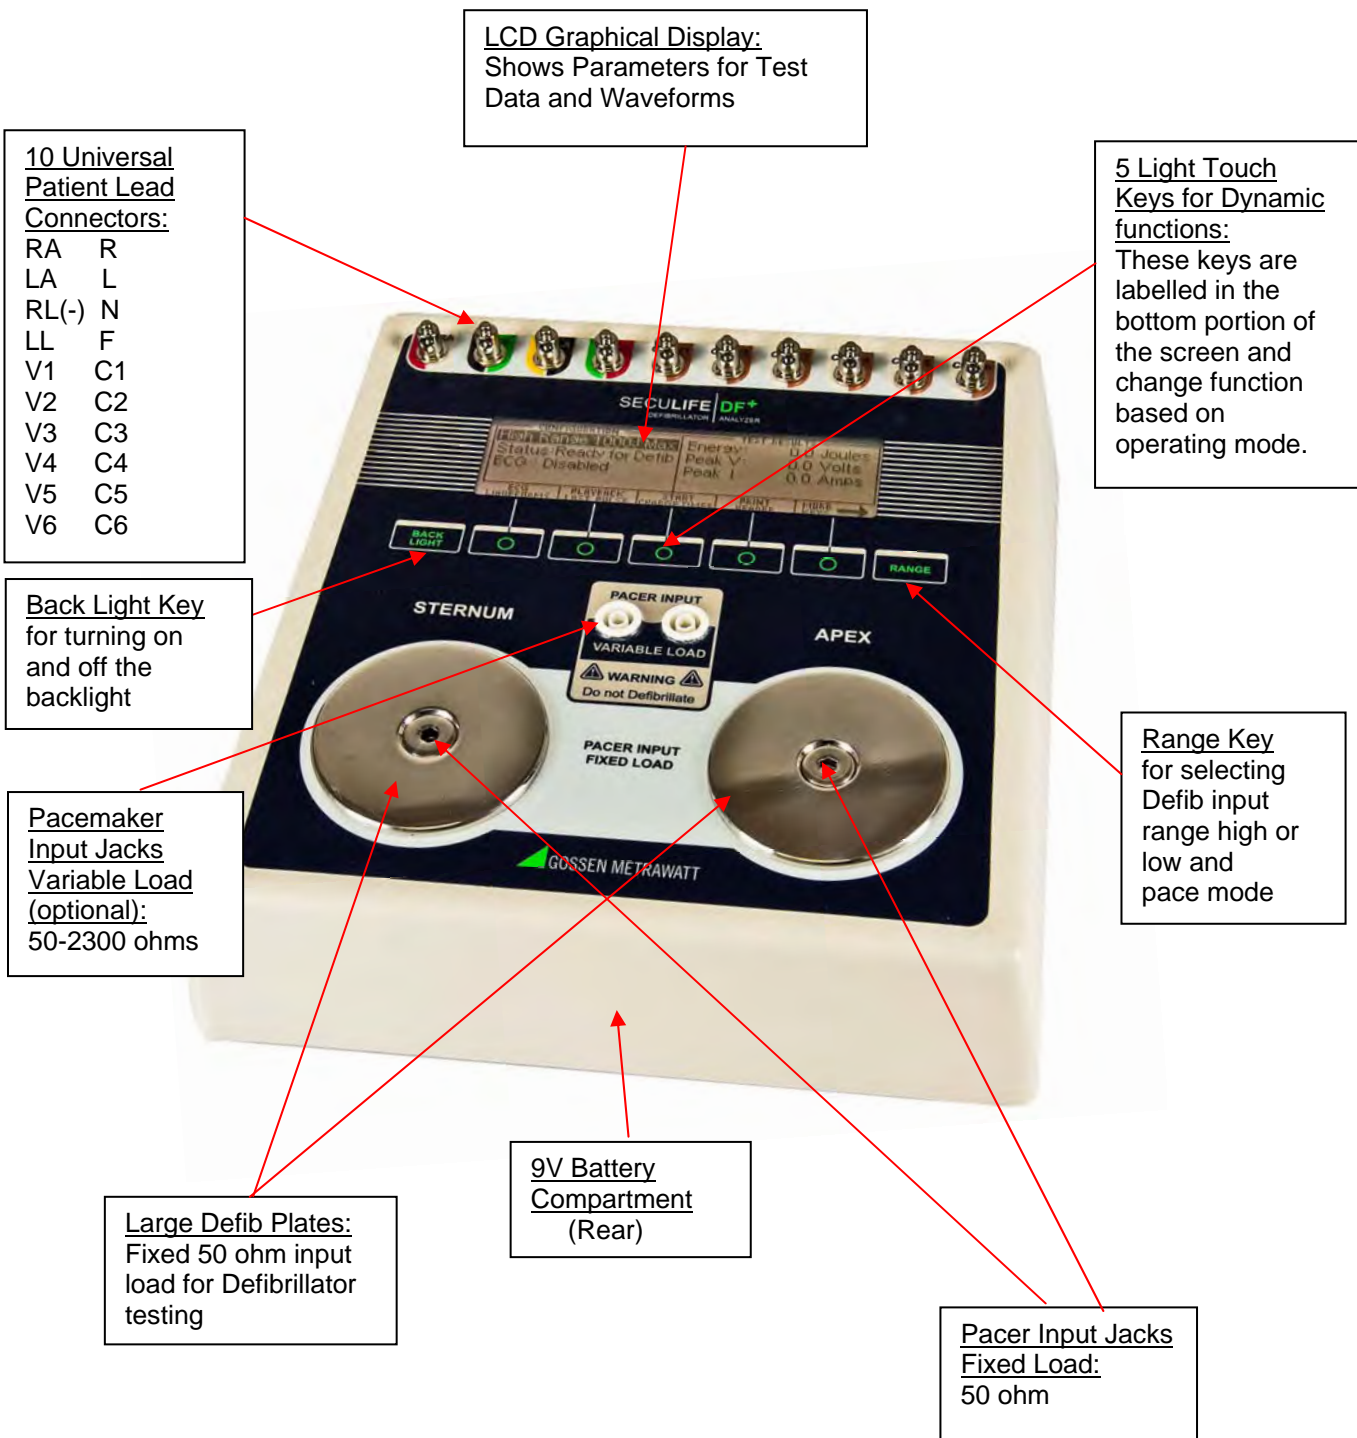

This section looks at the layout of the back and gives descriptions of the elements that are present.

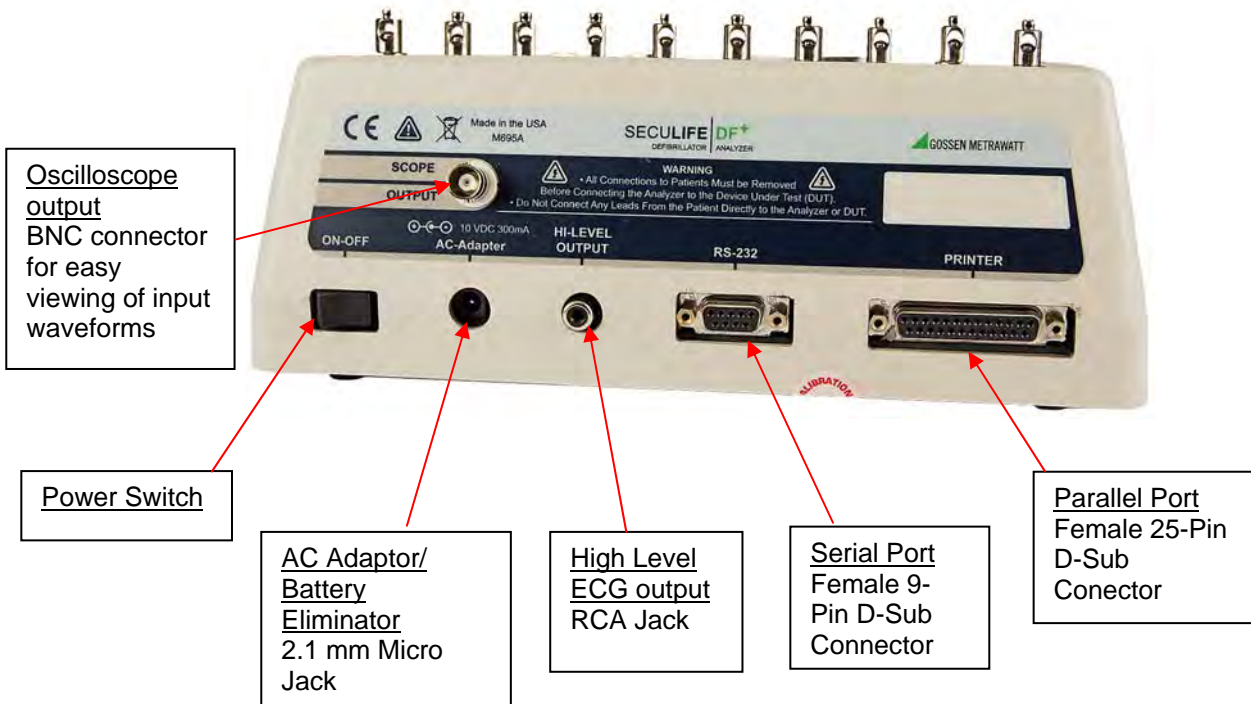


General Operation

The unit is controlled by 7 light touch keys. They allow the user to move around within the displayed parameters, select the desired options, choose a specific category and control the setup for the unit. When a key is depressed there is an audio click when it is accepted, or a razz tone if the key is invalid.

A large LCD graphics display with backlight provides the user with information about the current status of the device configuration options, test results and more. The display identifies the function of each key on a dynamic basis. As the operation mode changes, the key functions change to suit the operating mode.

Range Key


The  key scrolls through the ranges of the SECULIFE DF+ analyzer. Depressing the key will allow the user to select between High Defibrillator Range (1000J max), Low Defibrillator Range (50J max) and Pacemaker Range. The default mode on power up is High Defibrillator Range.

Backlight Key


The Graphic LCD display may be viewed with or without the backlight. Depressing any key will activate the backlight. However, since the backlight will drain the battery if left on, it will automatically shut off after a user programmable delay when running on battery power.

The  key is provided to toggle the backlight on or off at any time.

Function Keys

There are five  keys that are used to provide general operational control. The functions of the keys vary depending on the current screen. The section of the screen just above the key indicates its current meaning.

NOTE: Only functions that are available to the user will be visible at any given time.

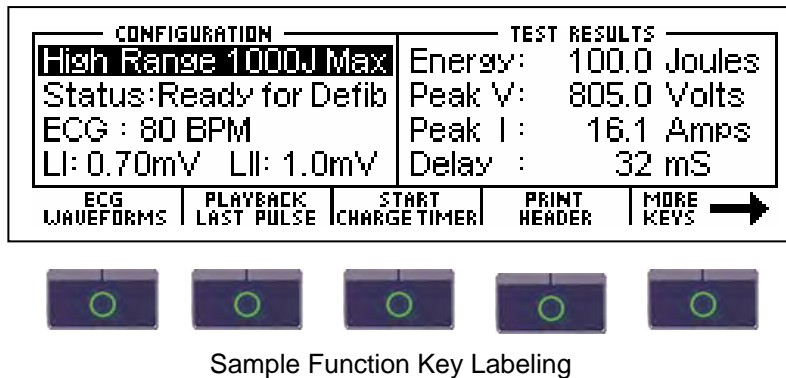

ECG Waveforms

The microprocessor has stored in its memory all of the digitalized waveforms. It sends the waveforms to a D/A converter, which generates an accurate analog representation. The waveform is then sent through resistor networks, developing the appropriate signals on the output terminals.

Universal Patient Lead Connectors

The 10 Universal Patient Lead Connectors allow for 12 lead ECG simulations. AHA and IEC color-coded labels are located on the face of the unit to aid in connecting the corresponding U.S. and International Patient Leads.

AHA Label	IEC Label	Description
RA	R	Right Arm
LA	L	Left Arm
RL	N	Right Leg (reference or ground)
LL	F	Left Leg
V1 V2 V3 V4 V5 V6	C1 C2 C3 C4 C5 C6	V Leads (V1-V6) (U.S. and Canada) also referred to as pericardial, precordial or unipolar chest leads Chest Leads (C1-C6) (International)

High Level Output (+)

A high level ECG output signal (200 X Amplitude Setting) is available on the RCA jack located on the rear of the unit.

Serial Port

A female 9-pin D-Sub connector is provided for the connection of the unit to a PC or laptop serial port (e.g. Com 1). This link is then used for either remote control or flash downloading of software upgrades.

Parallel Port

A female 25-pin D-Sub connector is provided for the connection of a printer via a Centronics parallel interface.

Oscilloscope Output

A BNC connector is provided to connect an oscilloscope to the unit. This output is a 200:1 attenuated version of the input to the Defibrillator Plates.

Power Switch

A rocker switch is provided on the rear of the unit to turn the power on and off.

Power Supply

The unit utilizes two 9 Volt Alkaline Batteries in the bottom battery compartments. When the unit detects a LOW BATTERY condition (10% Battery Life), a warning window will appear once per minute to alert the user.

Battery Eliminator

The unit has a 2.1 mm micro jack for connecting a 10-Volt AC battery eliminator. The adapter will power the unit, but will not charge the battery.

DEFIBRILLATOR ANALYZER

MAIN SCREEN

When the SECULIFE DF+ is first powered up, the Defibrillator Analyzer MAIN SCREEN will be displayed. This screen shows the current CONFIGURATION, the TEST RESULTS and the available FUNCTION KEYS. All defibrillator tests are run from the MAIN SCREEN. When the unit detects an input of greater than 100 Volts on the Defibrillator Plates (20 Volts in Low Range), it will automatically begin a test.

The default configuration is the High Range Defibrillator mode. This mode allows for a waveform of up to 1000 Joules to be analyzed.

The following is a sample screen for this mode:

CONFIGURATION		TEST RESULTS		
High Range 1000J Max	Energy: 100.0 Joules			
Status: Ready for Defib	Peak V: 805.0 Volts			
ECG : 80 BPM	Peak I : 16.1 Amps			
LI: 0.70mV LII: 1.0mV	Delay : 32 mS			
ECG WAVEFORMS	PLAYBACK LAST PULSE	START CHARGE TIMER	PRINT HEADER	MORE KEYS →

The **RANGE** key may be used to toggle the unit to the Low Range Defibrillator mode. This mode allows for waveforms up to 50 Joules to be analyzed. The Defibrillator Analyzer works the same in both ranges. The lower range simply provides for a higher resolution for pulses with smaller amplitudes.


The following is a sample screen for this mode:

CONFIGURATION		TEST RESULTS		
Low Range	50J Max	Energy:	20.4	Joules
Status:	Ready for Defib	Peak V:	367.5	Volts
ECG :	80 BPM	Peak I :	7.4	Amps
LI:	0.70mV	Delay :	394	mS
ECG WAVEFORMS	PLAYBACK LAST PULSE	START CHARGE/TIMER	PRINT HEADER	MORE KEYS →


NOTE: The **RANGE** key will also put the SECULIFE DF+ into the Transcutaneous Pacemaker Analyzer mode (See Pacemaker Analyzer section for more information).

CONFIGURATION

The CONFIGURATION section of the MAIN SCREEN displays the current setup of the unit.

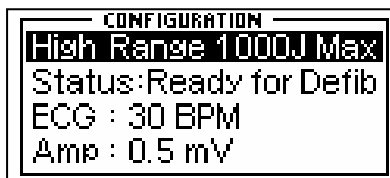

RANGE

The first line displays the range value for the pulse. It may be either 1000 Joules or 50 Joules max. This setting may be changed using the  key.

NOTE: This line also allows for the selection of the Pacer Analyzer. The  key will toggle to Pacer to put the unit into the Pacemaker Analyzer mode (See Pacemaker Analyzer section for more information).

STATUS

This line provides information about the current status of the analyzer.

ECG

This line displays the selection that is active on the ECG terminals. This setting may be changed in the ECG WAVEFORMS screen.

AMP

This line displays the amplitude that has been selected for the ECG terminals. This setting may be changed in the ECG WAVEFORMS screen.

TEST RESULTS

The TEST RESULTS section of the MAIN SCREEN displays the results of the last pulse. It will continue to be displayed until the power is turned off, another test is run or the range is changed.

TEST RESULTS	
Energy:	603.7 Joules
Peak V:	3565.0 Volts
Peak I:	71.3 Amps
Delay :	1205 mS

NOTE: The unit automatically starts a test when it sees a voltage greater than 100 Volts on the Defibrillator Plates (20 Volts in Low Range).

NOTE: Test results are immediately sent to the printer port as soon as the data is available.

ENERGY

This line displays the total energy of the last pulse.

PEAK V

This line displays the peak voltage of the last pulse.

PEAK I

This line displays the peak current of the last pulse.

DELAY

This line normally displays the delay from the peak of the R wave until the start of the Defib Energy pulse. The line is replaced by the CHARGE TIME if this test has been run (see START CHARGE TIMER SCREEN for more information).

CHG TIME


This line displays if the Charge Timer has been run. It shows the time required to charge the Device Under Test (DUT). This test is started with the

START CHARGE TIMER

 key.

FUNCTION KEYS

The FUNCTION KEYS section of the MAIN SCREEN displays the current functions of the keys found below the display. These keys allow for navigation to supporting screens and initiation of specific features.

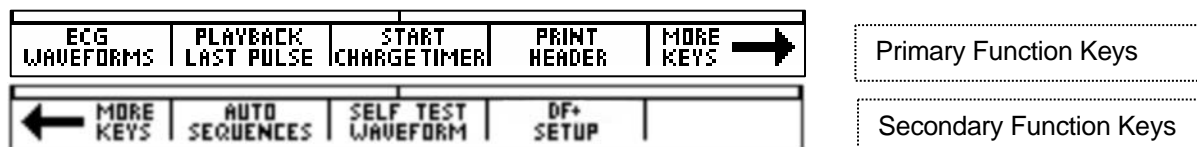

ECG WAVEFORMS

This key enters the ECG WAVEFORMS screen where all ECG parameters are set.

PLAYBACK LAST PULSE

This key enters the PLAYBACK LAST PULSE screen where a graphical representation of the last pulse may be viewed and sent out.

START CHARGE TIMER

This key brings up the CHARGE TIMER screen and starts the pre-warn timer. It is used to test the charge time for the defibrillator.

PRINT HEADER

This key sends the Report Header to the printer.

MORE KEYS

These keys toggle between the Primary and Secondary Function Keys.

AUTO SEQUENCES

This key brings up the AUTO SEQUENCE MENU, which is used to view or run the Auto Sequences stored in the unit.

SELF TEST WAVEFORM

This key sends an internal test pulse to the unit, allowing for the display of the results to give an indication that the system is working properly.

SECULIFE DF+ SETUP

This key brings up the SYSTEM CONFIGURATION SCREEN, which allows for adjusting the various system configuration parameters.

ECG WAVEFORMS SCREEN

The SECULIFE DF+ ECG output can be connected in 3, 5 or 12 lead configurations.

Pressing the **ECG WAVEFORMS** key from the MAIN SCREEN will allow the user to configure the waveform that is used for the ECG output.

The following is a sample of the ECG waveform configuration screen:

ECG GROUP	WAVEFORM
Disabled	None
NSR	30,40,45,60,80,90, 100,120,140,160, 180,200,220,240, 260,280,300 BPM
AED	Asystole
	Coarse Vfib
	Fine Vfib
	Multifocal Vtach 140
	Multifocal Vtach 160
	Polyfocal Vtach 140
	Polyfocal Vtach 160
	SupraVent Tach 90
Arrhythmias	Vfib
	Afib
	Second Deg Block
	RBBB
	PAC
	PVC Early
	PVC STD
	PVC R on T
	MF PVC
	Bigeminy
	Run of 5 PVC
	Vtach
	Performance
2, 2.5 Hz Triangle	
0.1,0.2,0.5,5,10,40,50,60,100 Hz Sine	
30, 60, 120 BPM Pulse	

ECG Configuration Screen

ECG Group: Disabled

Waveform: None

Amplitude : Lead I 0.70mV Lead II 1.0mV

▲ | ▼ | CHOICES | EXIT


AMPLITUDE


Lead I 0.35 mV Lead II 0.5 mV


Lead I 0.70 mV Lead II 1.0 mV

Lead I 1.05 mV Lead II 1.5 mV

Lead I 1.40 mV Lead II 2.0 mV

The ECG Group, Waveform and Amplitude can be selected using  to highlight the parameter and using **CHOICES** to open a drop down menu of all the options for the highlighted parameter.

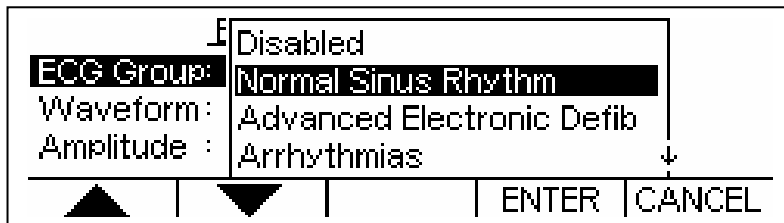

Use  to scroll to the desired option. Then **ENTER** is used to accept the new setting. The **CANCEL** key can be used to return to the ECG waveform configuration screen without making a new selection.

The **EXIT** key is used to return to the MAIN SCREEN.

The following is a brief description of how the SECULIFE DF+ simulates the available Arrhythmias:


Abbreviation	Arrhythmia	Description
Vent Fib – Fine	Ventricular Fibrillation	Irregular waveform with no real P-wave or clear R-R interval and a low signal level (Continuous)
Atrial Fib	Atrial Fibrillation	Absence of P-wave, irregular P-R interval rate and a high level signal (Continuous)
2nd Deg Heart Block	Second Degree Heart Block	80 BPM with increasing P-R interval for four beats (160, 220, 400, 470 ms) followed by a P wave without a QRS (Continuous)
Rt Bundle Branch Block	Right Bundle Branch Block	80 BPM with Normal P-wave and P-R interval but wider QRS complexes (Continuous)
PAC	Premature Atrial Contraction	NSR of 80 BPM with Periodic Abnormal 25% early P waves (PAC, 7 NSR) (Continuous)
PVC Early	Early Type 1 Premature Ventricular Contraction	NSR of 80 BPM with periodic left focus premature ventricular beats with 33% premature timing (PVC Type 1, 9 NSR) (Continuous)
PVC Std	Standard Type 1 Premature Ventricular Contraction	NSR of 80 BPM with periodic left focus premature ventricular beats with 20% premature timing (PVC Type 1, 9 NSR) (Continuous)
PVC R on T	R on T Type 1 Premature Ventricular Contraction	NSR of 80 BPM with periodic left focus premature ventricular beats with 65% premature timing, placing R on the previous T (PVC Type 1, 9 NSR) (Continuous)
Multifocal PVCS	Multifocal Premature Ventricular Contraction	NSR of 80 BPM with Type 1 and Type 2 PVCs (PVC Type 1, 2 NSR, PVC Type 2, 2 NSR) (Continuous)

Abbreviation	Arrhythmia	Description
Bigeminy	Bigeminal Rhythm	NSR of 80 BPM with every other beat a Type 1 PVC (Continuous)
Run of 5 PVCs	Run of 5 Premature Ventricular Contractions	NSR of 80 BPM with periodic group of 5 Type 1 PVCs (5 PVC Type 1, 36 NSR) (Continuous)
Vent Tach	Ventricular Tachycardia	160 BPM, No P-wave, Beats similar to Type 1 PVC (Continuous)

PLAYBACK LAST PULSE SCREEN

The SECULIFE DF+ can display a graphical representation of the last pulse. This screen may be accessed by pressing the **PLAYBACK LAST PULSE** key from the Defibrillator Analyzer MAIN SCREEN. The playback allows the user to view the Defibrillator pulse in a time-expanded form. Samples are stored internally at 0.1 ms intervals. The PLAYBACK LAST PULSE SCREEN shows these samples expanded by a time factor of 200.


In playback mode, the samples are shown on the display and sent out the ECG leads, Defibrillator Plates and the High Level output. The following is a sample of the waveform that is shown in the display:

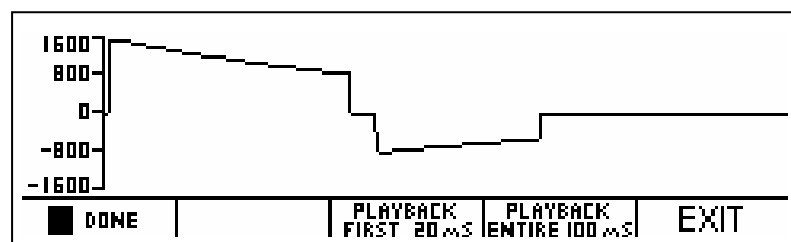


The scale shown on the screen is automatically adjusted to provide the maximum resolution available.

The **PAUSE** key can be used to pause the screen at any point while a pulse is being played back. This key replaces the **DONE** key when a pulse is being played back.

The **PLAY** key can be used to play (continue) the waveform if it has been paused. This key replaces the **PAUSE** key.


The  key starts a playback of only the first 20 ms of the waveform.

The  key starts a playback of the entire 100 ms of the waveform.


At any time, the  key or  key can be depressed to return to the MAIN SCREEN.

START CHARGE TIMER SCREEN


A special timer has been incorporated into the SECULIFE DF+ to analyze the charging circuit of the Device Under Test (DUT). The START CHARGE TIMER SCREEN can be accessed by pressing the **START CHARGE TIMER** key from the MAIN SCREEN. To synchronize the charge timer with the defibrillator charge time, a Pre-Warning Countdown period is started. When the timer reaches zero, the defibrillator charge should be initiated. The following is an example of the countdown timer:

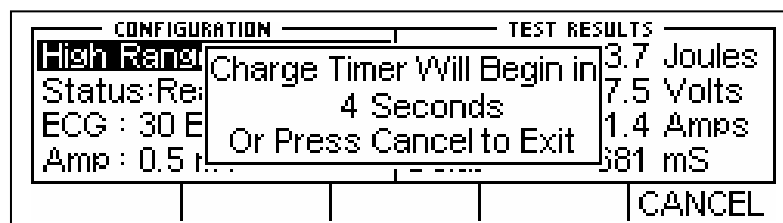

When the timer reaches zero, a beep will sound and the charge timer will begin counting up. The following is an example of the count up timer:

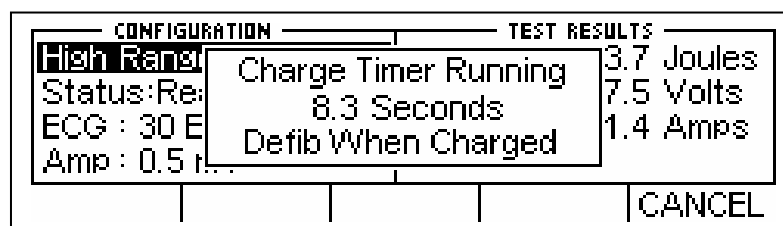

The DUT should be discharged as soon as it becomes charged. When the DUT is discharged, the timer will automatically stop. The display will show the results of the Defibrillator pulse analysis as well as the time required to charge the DUT:

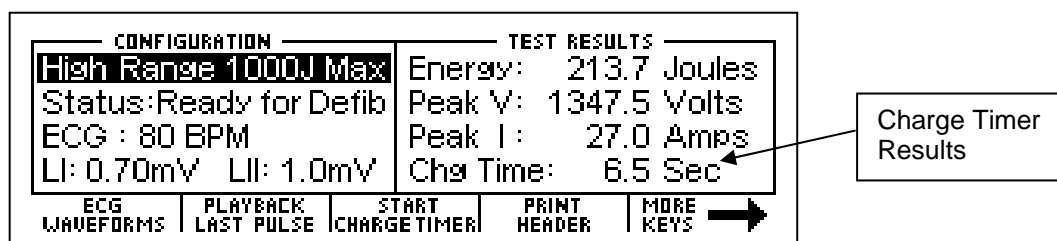

At any time, the **CANCEL** key can be depressed to end the timer and return to the MAIN SCREEN.

PRINT HEADER

The SECULIFE DF+ provides a header for recording test data as well as the results of each pulse that is discharged into the unit. Test results are immediately sent to the printer port as soon as the data is available. The header is sent by pressing the PRINT
HEADER key from the MAIN SCREEN.

The status line of the configuration section will indicate that the header has been sent to the printer.

CONFIGURATION		TEST RESULTS	
High Range 1000J Max	Energy: 213.7 Joules		
Status: Printing Header	Peak V: 1347.5 Volts		
ECG : 80 BPM	Peak I : 27.0 Amps		
LI: 0.70mV LII: 1.0mV	Chg Time: 6.5 Sec		
ECG WAVEFORMS	PLAYBACK LAST PULSE	START CHARGE TIMER	PRINT HEADER
			MORE KEYS →

The following is the print header and sample data that are used for the Defibrillator Analyzer mode.

```

                          Gossen Metrawatt
                    SECULIFE DF+ Defibrillator Analyzer

SECULIFE DF+ Serial Number: _____
Dut Manufacturer: _____
Dut Model: _____
Dut Serial Number: _____
Technician: _____
Location: _____

Date: _____

          +-----+          +-----+
          |         |          |         |
          |         |          |         |
          |         |          |         |
          +-----+          +-----+
          PASS              FAIL

Comments: _____
          _____
          _____

Test Data:
          Ecg      Ecg      Defib      Dut      +----- SECULIFE DF+ Measurements: -----+
Test#  Wave      Amp      Load      Setting | Energy Voltage Current Dely/ChgT |
-----+-----+-----+-----+-----+-----+-----+-----+
  1  None      1.0 mV    50ohm    _____J  112.5J  1085.0V  21.7A  0mS

```

NOTE: Printing the header also resets the test number printed on the data sheet.


NOTE: In the test results, the user must manually write the power setting of the DUT.

SELF TEST WAVEFORM


The SECULIFE DF+ has built in test waveforms that will give an indication that the system is working properly. The Self Test Waveform may be sent by pressing the **SELF TEST WAVEFORM** key from the MAIN SCREEN.

After the waveform has been sent, the results will be reflected in the test results section of the MAIN SCREEN and the PLAYBACK LAST PULSE SCREEN. The Self Test Waveform is not calibrated, but will provide a waveform that is approximately 125 Joules when configured for the High Range and 5 Joules when configured for the Low Range.

The following is an example of the MAIN SCREEN with the results of the Self Test Waveform:

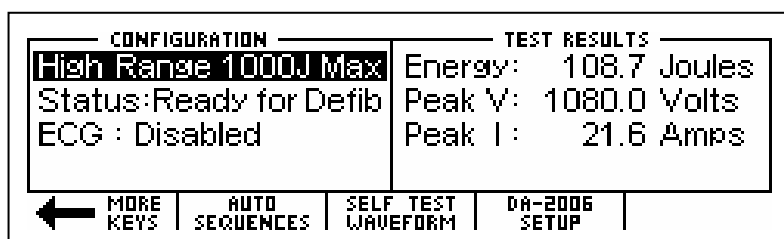

The following is an example of the PLAYBACK LAST PULSE SCREEN, showing a graphical representation of the Self Test Waveform:

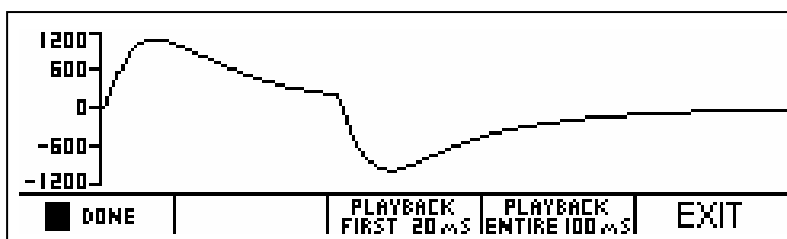

This page intentionally left blank.

RUNNING A DEFIBRILLATOR TEST

WARNING - CONNECTIONS

All connections to patients must be removed before connecting the Device Under Test (DUT) to the Analyzer. A serious hazard may occur if the patient is connected when testing with the Analyzer. Do not connect any leads from the patient directly to the Analyzer or DUT.

INTRODUCTION

The SECULIFE DF+ will analyze the pulse output of a monophasic or biphasic defibrillator. The primary measure of the output is the Energy that it contains. Other information deals with the maximum voltage and current as well as the pulse timing with respect to the R-wave.

The human body has characteristic impedance that may vary, but 50 ohms is used for comparative defibrillator testing. The SECULIFE DF+ has a large internal 50 ohm non-inductive, high-power resistor to simulate a human body. It is sized to accept repeated pulses at the maximum energy levels.

The energy contained in a pulse is determined mathematically based on the fact that the energy is defined as the integral of the power curve. The following formulas describe the basic computation:

$$\text{Energy} = E = \int P \, dt$$

$$\text{Power} = P = V^2 / R \Rightarrow \int E = V^2 / R \, dt = \int V^2 \, dt / R$$

This computation is implemented digitally by taking timed samples of the voltage every 100 μsec for 100 msec (1000 readings). Each value is then squared and divided by the resistance (50 ohms). The sum of these 1000 values times 10 is then the Energy in Joules (Watt Seconds) contained in the pulse.


DEFIBRILLATION TEST

The setup for a Defibrillation Test is dependent on the physical hardware involved. For the sake of this example we will assume a standard defibrillator with 5 lead ECG.

WARNING

This section is provided as a guide to familiarize the user with the SECULIFE DF+. It is not intended to provide the necessary test sequence for every Defibrillator. The user must consult the manufacturer's manual for each DUT to determine the correct test procedure to follow.

- (1) Connect ECG leads to the corresponding universal connector on the SECULIFE DF+. The connectors are marked with both the AHA and International color codes.
- (2) Turn on the SECULIFE DF+.
- (3) The unit will come up in the "High Range Defibrillator" mode. This range is used for normal adult testing.

NOTE: If it is desirable to run a test at 50 Joules or less with a peak voltage of 1000 Volts or less, the unit may be changed to the "Low Range Defibrillator" mode using the  key.
- (4) Select "Ventricular Fibrillation" from the ECG WAVEFORM SCREEN with an amplitude of 1 mV. This is necessary for most automatic defibrillators.
- (5) Place the Defibrillator Paddles on the SECULIFE DF+ contact plates. The APEX is on the right and the STERNUM is on the left.

NOTE: Reversing the paddles will not cause any damage to the unit or error in the energy reading. However, it will cause the polarity of the oscilloscope output and the playback waveform to be inverted.

- (6) Holding the paddles firmly in place, charge the Defibrillator and discharge it into the SECULIFE DF+.


<p style="text-align: center;">WARNING</p> <p>Observe all precautions noted by the Defibrillator Manufacturer when using the Defibrillator.</p>

- (7) The SECULIFE DF+ will automatically sense the voltage rise across the internal 50 ohm load and begin taking readings. After the sampling is done (100 ms) the unit will compute and display the results.

- a. The power pulse is available at the oscilloscope output in real time at 200:1 signal attenuation when in low range and 1000:1 signal attenuation when in high range.
- b. After the computation, the pulse is automatically played back at a 200:1 time base expansion (200 times slower) on both the ECG leads and the Paddle plates.

The signal level is 1 mV per 1000 Volts on Lead 1.

- c. At the same time, the test results are sent to the printer.

-
- (8) The Status line will change to indicate the various steps as they are being done.
- (9) At the end of the process the results are continuously displayed in the Test Results section of the MAIN SCREEN. They will remain there until another test is performed, the range is changed or the power is turned off.
- (10) The user may repeat the playback of the waveform at any time by changing to the PLAYBACK LAST PULSE SCREEN using the  key. In this screen the pulse may be viewed in 20 msec segments and paused for review.

NOTE: The pulse is sent to the ECG and Paddle outputs at the same time it is being displayed on the screen.

This page intentionally left blank.

CARDIOVERSION TEST

A Cardioversion Test is simply an energy test with special attention being given to the timing. The SECULIFE DF+ continuously monitors for the R-wave timing and displays, if possible, the delay between the R-wave and the pulse. In Cardioversion testing, the Defibrillator is set to deliver a pulse based on a specific delay after the R-wave.


WARNING

This section is provided as a guide to familiarize the user with the SECULIFE DF+. It is not intended to provide the necessary test sequence for every Defibrillator. The user must consult the manufacturer's manual for each DUT to determine the correct test procedure to follow.

- (1) Connect ECG leads to the corresponding universal connector on the SECULIFE DF+. The connectors are marked with both the AHA and International color codes.

- (2) Turn on the SECULIFE DF+.

- (3) The unit will come up in the "High Range Defibrillator" mode. This range is used for normal adult testing.

NOTE: If it is desirable to run a test at 50 Joules or less with a peak voltage of 1000 Volts or less, the unit may be changed to the "Low Range Defibrillator" mode using the  key.

- (4) Select the desired ECG Waveform and Amplitude to be tested from the choices on the ECG WAVEFORM SCREEN.

NOTE: The selected waveform must contain a QRS complex.

- (5) Set the Defibrillator to Synchronized Cardioversion mode.

- (6) Place the Defibrillator Paddles on the SECULIFE DF+ contact plates. The APEX is on the right and the STERNUM is on the left.

NOTE: Reversing the paddles will not cause any damage to the unit or error in the energy reading. However, it will cause the polarity of the oscilloscope output and the playback waveform to be inverted.


- (7) Holding the paddles firmly in place, charge the Defibrillator and discharge it into the SECULIFE DF+.

WARNING

**Observe all precautions noted by the Defibrillator
Manufacturer when using the Defibrillator.**

-
- (8) The SECULIFE DF+ will automatically sense the voltage rise across the internal 50 ohm load and begin taking readings. After the sampling is done (100 ms) the unit will compute and display the results.
- The power pulse is available at the oscilloscope output in real time at 200:1 signal attenuation when in low range and 1000:1 signal attenuation when in high range.
 - After the computation, the pulse is automatically played back at a 200:1 time base expansion (200 times slower) on both the ECG leads and the Paddle plates. The signal level is 1 mV per 1000 Volts on Lead 1.
 - At the same time, the test results are sent to the printer.
- (9) The Status line will change to indicate the various steps as they are being done.
- (10) At the end of the process the results are continuously displayed in the Test Results section of the MAIN SCREEN. They will remain there until another test is performed, the range is changed or the power is turned off.

NOTE: Special note should be made of the "Delay: xxx msec" line in the results. This will show the delay between the peak of the R-wave and the start of the Pulse.

The user may repeat the playback of the waveform at any time by changing to the PLAYBACK LAST PULSE SCREEN using the  key. In this screen the pulse may be viewed in 20 msec segments and paused for review.

NOTE: The pulse is sent to the ECG and Paddle outputs at the same time it is being displayed on the screen.


CHARGE TIME TEST

The charging time of a Defibrillator is nothing more than a measurement of the time required for the Defibrillator to charge. It is used to test the battery, charging circuitry and capacitor.

The SECULIFE DF+ provides a simple way to start and stop the timer. It also records the results.

WARNING

This section is provided as a guide to familiarize the user with the SECULIFE DF+. It is not intended to provide the necessary test sequence for every Defibrillator. The user must consult the manufacturer's manual for each DUT to determine the correct test procedure to follow.

- (1) Turn on the SECULIFE DF+.
- (2) The unit will come up in the "High Range Defibrillator" mode. This range is used for normal adult testing.
- (3) Set the Defibrillator to its maximum power setting.
- (4) Depress the  key.

- (5) While the Pre-Warning Countdown is running, place the Defibrillator Paddles on the SECULIFE DF+ contact plates. The APEX is on the right and the STERNUM is on the left.

NOTE: Reversing the paddles will not cause any damage to the unit or error in the energy reading. However, it will cause the polarity of the oscilloscope output and the playback waveform to be inverted.

- (6) Holding the paddles firmly in place, wait until the Pre-Warning Countdown equals zero and then immediately start charging the Defibrillator.

- (7) As soon as the DUT is fully charged, discharge it into the SECULIFE DF+.

WARNING

Observe all precautions noted by the Defibrillator Manufacturer when using the Defibrillator.

- (8) At the end of the process the results are continuously displayed in the Test Results section of the MAIN SCREEN. They will remain there until another test is performed, the range is changed or the power is turned off.

NOTE: The last line in the Test Results section of the screen will show

“Chg Time: xxx.x sec”

SHOCK ADVISORY ALGORITHM TEST

The Shock Advisory Algorithm Test works with the analysis and prompting functions on automatic and semiautomatic Defibrillators. These circuits look at ECG waveforms and prompt the user to “Shock” or “No Shock” based on national and international guidelines. The following table outlines these guidelines:

SHOCK ADVISORY ALGORITHM TEST	
ECG SIGNALS	ACTION
Asystole	No Shock
Supra Ventricular Tachycardia @ 90 BPM	No Shock
Polyfocal Ventricular Tachycardia @ 140 BPM	No Shock
Multifocal Ventricular Tachycardia @ 140 BPM	No Shock
Coarse Ventricular Fibrillation	Shock
Fine Ventricular Fibrillation	Shock
Polyfocal Ventricular Tachycardia @ 160 BPM	Shock
Multifocal Ventricular Tachycardia @ 160 BPM	Shock

WARNING

This section is provided as a guide to familiarize the user with the SECULIFE DF+. It is not intended to provide the necessary test sequence for every Defibrillator. The user must consult the manufacturer’s manual for each DUT to determine the correct test procedure to follow.

- (1) Connect ECG leads to the corresponding universal connector on the SECULIFE DF+. The connectors are marked with both the AHA and International color codes.

- (2) Turn on the SECULIFE DF+.

- (3) The unit will come up in the “High Range Defibrillator” mode. This range is used for normal adult testing.

- (4) Select the desired AED Waveform and Amplitude to be tested from the choices on the ECG WAVEFORM SCREEN.

- (5) Set the Defibrillator to analyze the ECG waveform in the automatic or semiautomatic mode.

- (6) Observe and record the response of the Defibrillator to the various waveforms.

TRANSCUTANEOUS PACEMAKER ANALYZER

The SECULIFE DF+ can analyze pacemaker pulses as well as determine Refractory periods and Sensitivity levels of on-demand pacemakers. For maximum versatility, the SECULIFE DF+ has 26 internally selectable pacemaker loads ranging from 50 ohms to 2300 ohms. The SECULIFE DF+ can also test the noise immunity of the DUT by generating a 50 or 60 Hz noise waveform with amplitude up to 100 mV. For sensitivity testing, the SECULIFE DF+ can output a Square, Triangle or Haversine waveform with widths ranging from 10ms to 200ms. The input circuitry of the SECULIFE DF+ is protected against damage in the case of an accidental defibrillator discharge into the Pacemaker Input terminals.

The  key is used to change to the Pacemaker Analyzer mode.

PACE MAIN SCREEN

The Pacemaker Analyzer MAIN SCREEN shows the current CONFIGURATION, the TEST RESULTS and the available FUNCTION KEYS.


The following is a sample of the PACE MAIN SCREEN:

CONFIGURATION			TEST RESULTS	
Pace	: DO NOT DEFIB		Rate	: 80 ppm
Load	: 50 ohm		Width	: 39.8 mS
Noise	: None		Amp	: 18.2 mA
Wave	: 40 mS Square		Energy	: 0.6 mJ
PACE MODE	SENSITIVITY	REFRACTORY	TOGGLE	MORE
SETUP	TEST	PERIOD TEST	TEST RESULTS	KEYS →

NOTE: The Test Results section of the PACE MAIN SCREEN contains eight lines of data that can be toggled to view the first 4 lines or the second 4 lines (See TEST RESULTS section of manual for more information).

CONFIGURATION

The CONFIGURATION section of the PACE MAIN SCREEN displays the current setup of the unit.

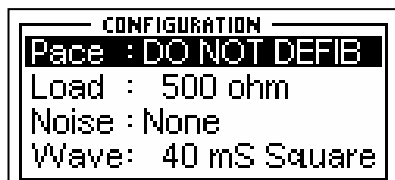

LOAD

This line displays the selected load. This setting may be changed in the PACE MODE SETUP screen.

The load choice determines what impedance is used at the pacemaker input as well as whether the unit uses the Pacer Input Terminals or the Defibrillator Plate Input Terminals.

NOISE


This line displays the selected noise output. This setting may be changed in the PACE MODE SETUP screen.

WAVE

This line displays the selected output waveform. This setting may be changed in the PACE MODE SETUP screen. The selected waveform is the output to the pacer on the ECG Terminals, Pacer Terminals and Defibrillator Plate Terminals.

TEST RESULTS

The TEST RESULTS section of the PACE MAIN SCREEN displays the results of the last test. It will continue to be displayed until the power is turned off or another test is run.

The Test Results section of the PACE MAIN SCREEN contains eight lines of data that can be toggled to view the first 4 lines or the second 4 lines by pressing the  key.

TEST RESULTS	
Rate :	80 ppm
Width :	19.9 mS
Amp :	92.3 mA
Energy:	32.0 mJ

TEST RESULTS	
Sens.Pads:	1.62 mV
Sens.ECG :	0.21 mV
Paced RP :	270 mS
Sensed RP:	97 mS

RATE

This line displays the rate of the pacemaker pulse that is present at the selected load.

WIDTH

This line displays the width of the pacemaker pulse that is present at the selected load.

AMP

This line displays the current of the pacemaker pulse that is present at the selected load.

ENERGY

This line displays the energy of the pacemaker pulse that is present at the selected load.

SENS PADS

This line displays the sensitivity at the pads for the selected waveform during the last Sensitivity Test.

SENS ECG

This line displays the sensitivity at the ECG leads for the selected waveform during the last Sensitivity Test.

PACED RP

This line displays the paced refractory period detected at the selected load during the last Refractory Period Test.

SENSED RP

This line displays the sensed refractory period detected at the selected load during the last Refractory Period Test.

FUNCTION KEYS

The FUNCTION KEYS section of the PACE MAIN SCREEN displays the current functions of the keys found below the display. These keys allow for navigation to supporting screens and initiation of specific features.

PACE MODE SETUP	SENSITIVITY TEST	REFRACTORY PERIOD TEST	TOGGLE TEST RESULTS	MORE KEYS →
--------------------	---------------------	---------------------------	------------------------	----------------

Primary Function Keys

← MORE KEYS	PRINT MENU	PLAYBACK LAST PULSE	AUTO SEQUENCES	DF+ SETUP
----------------	---------------	------------------------	-------------------	--------------

Secondary Function Keys

PACE MODE SETUP

This key enters the PACE MODE SETUP SCREEN where all pace parameters are chosen.

SENSITIVITY TEST

This key activates a Sensitivity Test.

REFRACTORY PERIOD TEST

This key activates a Refractory Period Test.

TOGGLE TEST RESULTS

This key toggles the test result section to view the first 4 lines or the second 4 lines of data.

MORE KEYS

These keys toggle between the Primary and Secondary Function Keys.

PRINT MENU

This key enters the PRINT SCREEN that allows the printing of the header or the test data.

PLAYBACK LAST PULSE

This key enters the PLAYBACK LAST PULSE screen where a graphical representation of the last pulse may be viewed and sent out.

AUTO SEQUENCES

This key brings up the AUTO SEQUENCE MENU, which is used to view or run the Auto Sequences stored in the unit.

SECULIFE DF+ SETUP


This key brings up the SYSTEM CONFIGURATION SCREEN, which allows for adjusting the various system configuration parameters.


PACER MODE SETUP SCREEN

The SECULIFE DF+ can be configured to run a large number of tests under various load conditions. This screen is used to configure the unit for these tests. The pacemaker configuration screen is accessed by pressing the **PACE MODE SETUP** key from the PACE MAIN SCREEN. In this screen, the user can select the desired Load, the output Noise waveform, the Sensitivity Test waveform, and the Pacemaker Pulse Filter.

The following is a sample of the Pacemaker configuration screen:

LOAD	<div style="border: 1px solid black; padding: 5px;"> Load : 100 ohm Noise : None Wave: 40 mS Square Pacemaker Pulse Filter: 0.0 mS <hr/> <div style="display: flex; justify-content: space-between; align-items: center;"> ▲ ▼ CHOICES EXIT </div> </div>		
Defib Plates Input (50Ω) 50 ohm 100 ohm 150 ohm 200 ohm 200 ohm 300 ohm 400 ohm 500 ohm 600 ohm 700 ohm 800 ohm 900 ohm 1000 ohm 1100 ohm 1200 ohm 1300 ohm 1400 ohm 1500 ohm 1600 ohm 1700 ohm 1800 ohm 1900 ohm 2000 ohm 2100 ohm 2200 ohm 2300 ohm Open	NOISE	WAVEFORM	PULSE FILTER
	10 mV 50 Hz 9 mV 50 Hz 8 mV 50 Hz 7 mV 50 Hz 6 mV 50 Hz 5 mV 50 Hz 4 mV 50 Hz 3 mV 50 Hz 2 mV 50 Hz 1 mV 50 Hz NONE 1 mV 60 Hz 2 mV 60 Hz 3 mV 60 Hz 4 mV 60 Hz 5 mV 60 Hz 6 mV 60 Hz 7 mV 60 Hz 8 mV 60 Hz 9 mV 60 Hz 10 mV 60 Hz	10 ms Square 25 ms Square 40 ms Square 100 ms Square 200 ms Square 10 ms Triangle 25 ms Triangle 40 ms Triangle 100 ms Triangle 200 ms Triangle 10 ms SSQ 25 ms SSQ 40 ms SSQ 100 ms SSQ 200 ms SSQ	0.0 – 2.0 mS

These settings can be selected using  to highlight the parameter and using **CHOICES** to open a drop down menu of all the options for the highlighted parameter.

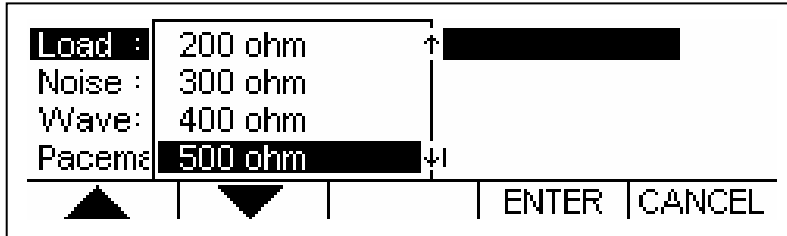


Use  to scroll to the desired option. Then **ENTER** is used to accept the new setting.

The **CANCEL** key can be used to return to the Pacemaker configuration screen without making a new selection.

The **EXIT** key is used to return to the PACE MAIN SCREEN.

PACEMAKER PULSE FILTER - This filter eliminates noise pulses from being detected as pacemaker pulses. Any pulses that have a width less than the Pacemaker Pulse Filter setting will be ignored. When set to 0.0, the filter is disabled. When the filter is ON, an indicator will show "FILTER ON" in the main pacemaker screen.

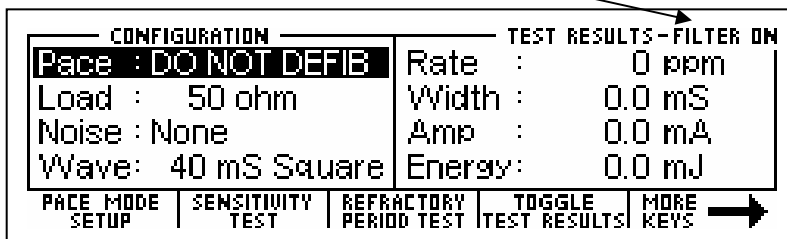

SENSITIVITY TEST

The Sensitivity Test is used to determine the smallest waveform that the pacemaker can detect. For this test, the selected waveform is generated outside of the refractory period of the pacemaker. The SECULIFE DF+ uses a successive approximation approach to determine the smallest output waveform that can be detected by the pacemaker. The Sensitivity Test may be initiated by pressing the **SENSITIVITY TEST** key from the PACE MAIN SCREEN.

WARNING

This section is provided as a guide to familiarize the user with the SECULIFE DF+. It is not intended to provide the necessary test sequence for every Pacemaker. The user must consult the manufacturer's manual for each DUT to determine the correct test procedure to follow.

While this test is running, the following display will show the progress of the test:

CONFIGURATION	TEST RESULTS
Pace : DC	Sensitivity Test Running 0.00 mV
Load : 50	0.00 mV
Noise : Nor	Please Wait 0 mS
Wave: 40	Or Press Cancel to Exit 0 mS
	CANCEL


At any time, the **CANCEL** key can be depressed to stop the test and return to the PACE MAIN SCREEN.

At the end of the test, the display will show the pacemaker amplitude sensitivity at the Pacer Terminals and the ECG Terminals.

CONFIGURATION		TEST RESULTS		
Pace : DO NOT DEFIB		Sens.Pads :	0.71 mV	
Load : 50 ohm		Sens.ECG :	0.09 mV	
Noise : None		Paced RP :	0 mS	
Wave: 40 mS Square		Sensed RP:	0 mS	
PACE MODE SETUP	SENSITIVITY TEST	REFRACTORY PERIOD TEST	TOGGLE TEST RESULTS	MORE KEYS →

REFRACTORY PERIOD TEST

For on-demand pacemakers, the pacemaker should ignore any ECG activity after a pacer pulse for a specific period of time. This time period is known as the Refractory Period. The Paced Refractory Period is the time after the pacemaker pulse that ECG activity is ignored. If an ECG pulse is present inside the refractory period, it is ignored. If an ECG pulse is detected outside of the refractory period, the pacemaker will re-synchronize to the sensed ECG pulse. For each sensed ECG pulse, there is a second refractory period. This is known as the Sensed Refractory Period. It is the period of time after the sensed ECG pulse that ECG activity is ignored.

The Refractory Period Test may be initiated by pressing the  key from the PACE MAIN SCREEN.

WARNING

This section is provided as a guide to familiarize the user with the SECULIFE DF+. It is not intended to provide the necessary test sequence for every Pacemaker. The user must consult the manufacturer's manual for each DUT to determine the correct test procedure to follow.

While the Refractory Period test is running, the display will indicate the progress of the test:

CONFIGURATION	TEST RESULTS
Pace : DO	Refractory Test Running
Load : 50	[Progress Bar]
Noise : Nor	Please Wait
Wave: 40	Or Press Cancel to Exit
	0 ppm 0.0 mS 0.0 mA 0.0 mJ
	CANCEL

NOTE: It is important that the pulse rate does not change for the duration of the Refractory Test.


At any time, the **CANCEL** key can be depressed to stop the test and return to the PACE MAIN SCREEN.

When the test is completed, the display will update with the Paced Refractory Period and Sensed Refractory Period in the Test Results.


CONFIGURATION		TEST RESULTS		
Rate : DO NOT DEFIB		Sens.Pads :	0.71 mV	
Load : 50 ohm		Sens.ECG :	0.09 mV	
Noise : None		Paced RP :	245 mS	
Wave : 40 mS Square		Sensed RP :	200 mS	
PACE MODE SETUP	SENSITIVITY TEST	REFRACTORY PERIOD TEST	TOGGLE TEST RESULTS	MORE KEYS →

PRINT MENU SCREEN

The SECULIFE DF+ allows the user to print the latest Pacemaker Analysis data or a header.


The PRINT MENU SCREEN is accessed by pressing the  key from the PACE MAIN SCREEN.

The following is an example of the print menu screen:

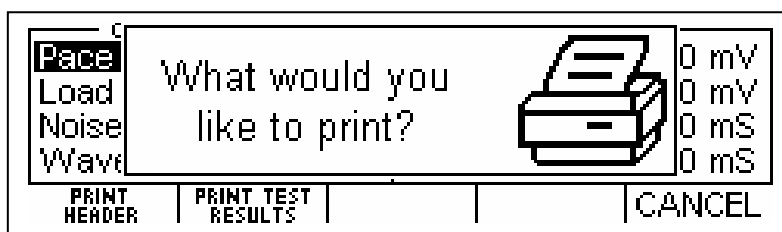


The header is sent by pressing the  key.

The test data is sent by pressing the  key.


The  key can be depressed to return to the PACE MAIN SCREEN.

PLAYBACK LAST PULSE SCREEN



The SECULIFE DF+ can display a graphical representation of the last pulse. This screen may be accessed by pressing the  key from the PACE MAIN SCREEN.

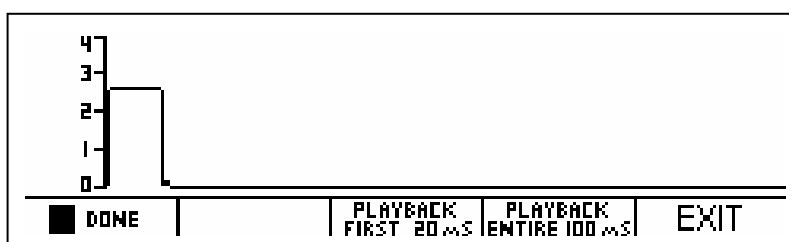

The playback allows the user to view the Pacemaker pulse in a time-expanded form. Samples are stored internally at 0.1 ms intervals. The PLAYBACK LAST PULSE SCREEN shows these samples expanded by a time factor of 200.


In playback mode, the samples are shown on the display and sent out the ECG leads, Defibrillator Plates, and the High Level output. The following is a sample of the waveform that is shown in the display:






The scale shown on the screen is automatically adjusted to provide the maximum resolution available.

The  key can be used to pause the screen at any point while a pulse is being played back. This key replaces the  key when a pulse is being played back.

The  key can be used to play (continue) the waveform if it has been paused. This key replaces the  key.

The  key starts a playback of only the first 20 ms of the waveform.

The  key starts a playback of the entire 100 ms of the waveform.

At any time, the  key or  key can be depressed to return to the MAIN SCREEN.

MESSAGES

INPUT OVERLOAD

The “Warning Input Overload Check Range” message can display during Defibrillator testing. The range should be checked to see if it should be changed to High Range for the current Joule setting.

CONFIGURATION		TEST RESULTS	
Low Range 50J Max Status: Ready for Defib ECG : Disabled	En Pe Pe	WARNING Input Overload Check Range	PS S IS
ECG WAVEFORMS	PLAYBACK LAST PULSE	START CHARGE TIMER	PRINT HEADER
			MORE KEYS →

NO PULSE

The “Test Cancelled No Pulse for 3 seconds” message can display during Refractory or Sensitivity Pacer testing. The settings should be checked and the test rerun.

CONFIGURATION		TEST RESULTS	
Pace : DO	Test Cancelled	0 ppm	
Load : 10	No Pulse for 3 seconds	0.0 mS	
Noise : Nor	Check Settings and retry	0.0 mA	
Wave: 40	Or Press Cancel to Exit	0.0 mJ	
		RETRY	CANCEL

SENSITIVITY TOO HIGH

The “Test Cancelled DUT Sensitivity too high” message can display during Pacer testing.

This happens when the Pacemaker does not detect the pulse generated by the SECULIFE DF+. It could be that it is connected improperly or set to Async mode. This can occur during either the Sensitivity or Refractory test modes.

CONFIGURATION		TEST RESULTS	
Pace : DO	Test Cancelled	0 ppm	
Load : 10	DUT Sensitivity too high	0.0 mS	
Noise : Nor	Reduce Sens and retry	0.0 mA	
Wave: 40	Or Press Cancel to Exit	0.0 mJ	
			RETRY CANCEL

LOW BATTERY

This message indicates that the batteries are low and should be replaced.

CONFIGURATION		TEST RESULTS	
High Range	LOW BATTERY 7% Life Remaining	0.0 Joules	
Status: Pleas		0.0 Volts	
ECG : Disabl		0.0 Amps	
ECG WAVEFORMS	PLAYBACK LAST PULSE	START CHARGE TIMER	PRINT HEADER MORE KEYS →

EXITING AUTO SEQUENCE TESTING

The “Exit Auto Sequence Test All Data Will be Lost!” message will display in the Auto Sequencing Mode when is pushed. If the data is needed, it should be printed prior to exiting.

		TEST RESULTS	
LifePak 8P	Exit AutoSequence Test	0 ppm	
Set Pacer	All Data Will be Lost!	0.0 mS	
Press Star	Are You Sure?	0.0 mA	
PaceRP:		0.0 mJ	
			YES NO

This page intentionally left blank.

POWER UP SETTINGS

The SECULIFE DF+ allows the user to tailor the settings that the unit will have on Power Up. The “Power Up With” parameter in the System Setup Menu allows for the selection of either Default or Custom selections.

DEFAULT

If this option is selected the following settings will be used every time the unit is turned on.

Range – Defib, High Range mode

ECG – Output Disabled

Pacemaker Load – 100 ohm

Pacemaker Noise Waveform- None

Pacemaker Output Waveform – 40 ms Square wave.

CUSTOM

If this option is selected, the user may save a unique set of default parameters and the unit will recall them every time the power is turned on.

SET CURRENT AS CUSTOM


The user simply configures the unit to the desired default conditions, selects this option and presses . The current configuration is then saved as the Custom Power up values.

This page intentionally left blank.

AUTO SEQUENCE FUNCTION

The SECULIFE DF+ allows the user run up to 50 pre-programmed sequences of tests (Auto Sequences). The tests are configured with an easy to use PC program. Each test can be configured to test Defibrillator, Transcutaneous Pacemaker or both. (For programming Auto Sequences, see the Auto Sequence Programming section).

Once configured, the tests are then downloaded to the SECULIFE DF+ unit through the RS232 serial interface.

The AUTO SEQUENCE SCREEN is accessed using the  key.




Use arrows to find
Auto Sequence

Sequence Type:
Defib and Pacer

▲	▼	VIEW	RUN	EXIT
---	---	------	-----	------

AUTO SEQUENCES

- LifePak 4
- LifePak 5
- LifePak 6
- LifePak 6S
- LifePak 8P
- LifePak 9P
- LifePak 9PM
- LifePak 10
- LifePak 10P
- LifePak 10PM
- HP 78660A
- HP XLPM
- Nihon Kohden 7000
- Laerdal HS 2000
- Marquette 1500PM
- Zoll PD 2000
- Zoll M-Series DSW
- Zoll AED Plus
- Blank Tests 20-50

In this menu, the  keys are used to select the desired test. The  key can be used to enter the VIEW MODE which will allow the user to view the programmed test options of the selected test. The  key will run the selected test and enter the RUN MODE which will step the technician through the programmed test as well as identify whether each step has passed or failed based upon the pre-programmed test limits that are part of each Auto Sequence.

The following table shows the possible test sequence with the details and options that can be selected using the PC program:

Test	Description	Fields	Options
Defibrillator Test Sequence			
Defib Energy Tests	Measures defibrillator discharge energy	Steps	1-20 xxx Joules
		Energy Level Limits	0-99%
		VFIB ECG Output	yes/no
Maximum Energy Test	Measures time required for defibrillator to charge to maximum energy	Do Test?	yes/no
		Energy Level Limits	xxx Joules
		Max Allowed Charge Time	x sec
Cardioversion Tests	Measures Cardioversion Delay	Steps	1-3 xxx Joules
		Energy Level Limits	0-99%
ECG Performance Test	Tests defibrillator ECG input	Steps	Up to 10
		Waveform Outputs and Amplitudes	x Waveform Group x Waveform Lead II = x.x mV
Pacemaker Test Sequence			
Pulse Rate and Amplitude Tests	Measures Pacemaker Pulse Rate and Amplitude	Steps	1-20
		Pulse Rate, Pulse Amplitude and Load settings	xxx ppm xx mA xxx ohms
		Limits for Rate and Amplitude	0-99%
Asynchronous Test	Tests Pacemaker Asynchronous Mode	Do Test?	yes/no
		Pulse Rate and Load	xxx ppm xxx ohms
Demand Mode Tests	Measures Pacemaker Sensitivity at Pacemaker Pads and ECG leads	Steps	1-5
		Pulse Rate, Load and Output Waveform	xxx ppm xxx ohms x Waveform
Refractory Test	Measures Paced Refractory Period and Sensed Refractory Period	Do Test?	yes/no


VIEW MODE

The VIEW MODE allows the user to look at the test configuration. Each test setting will be shown, as well as the test limits that identify a valid or invalid test result. The screens that are displayed in the VIEW MODE are determined by the Auto Sequence selected on the AUTO SEQUENCE SCREEN and its configuration as defined with the PC program.

The following screens are examples of what could be shown in the VIEW MODE if all test options are selected:

NOTE: If any particular test option is disabled using the PC Program, it will not be shown in the VIEW MODE.

DEFIBRILLATOR ENERGY TESTS:

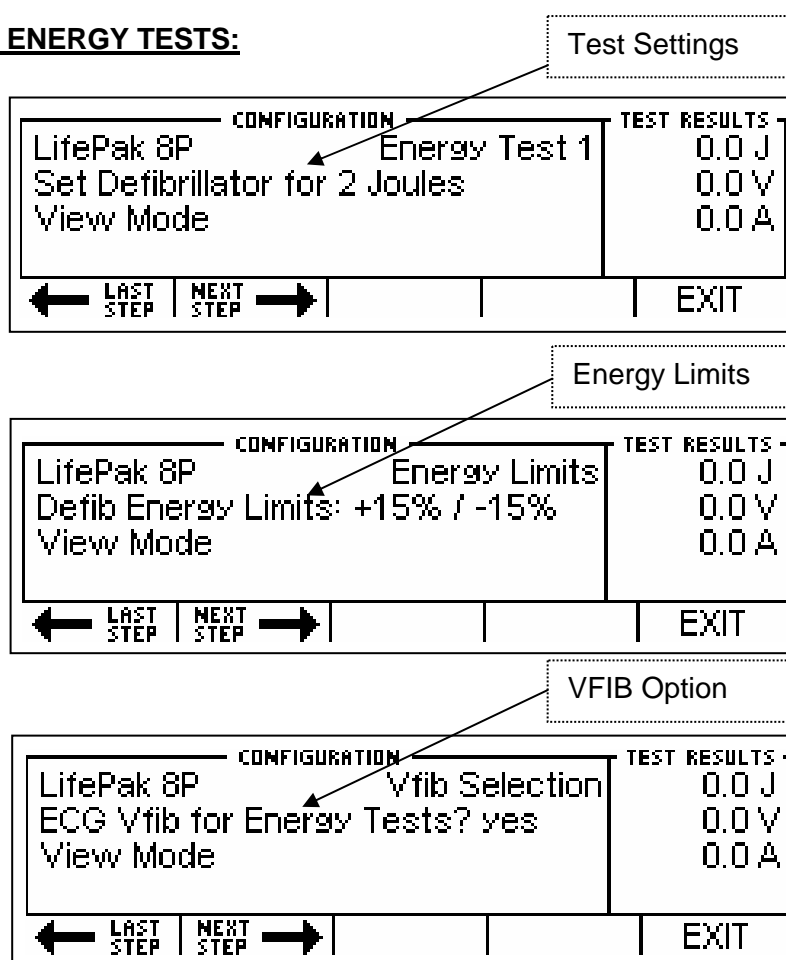

DEFIBRILLATOR MAXIMUM ENERGY TESTS:

Max Energy

CONFIGURATION	TEST RESULTS
LifePak 8P	MaxE Chg Time 0.0 J
Set Defibrillator for 360 Joules	0.0 V
View Mode	0.0 A
	0.0 S
← LAST STEP NEXT STEP →	EXIT

Max Energy Test Limits

CONFIGURATION	TEST RESULTS
LifePak 8P	MaxE Chg Time 0.0 J
Energy Limits: 338 to 382 Joules	0.0 V
View Mode	0.0 A
	0.0 S
← LAST STEP NEXT STEP →	EXIT


DEFIBRILLATOR CARIOVERSION TESTS:

Test Settings




CONFIGURATION	TEST RESULTS
LifePak 8P	Crdvrsn Test 1 0.0 J
Set Defibrillator for 100 Joules	0.0 V
View Mode	0.0 A
	0 mS
← LAST STEP NEXT STEP →	EXIT

Test Limits


CONFIGURATION	TEST RESULTS
LifePak 8P	Crdvrsn Limits 0.0 J
Cardioversion Limit +12% / -12%	0.0 V
View Mode	0.0 A
	0 mS
← LAST STEP NEXT STEP →	EXIT

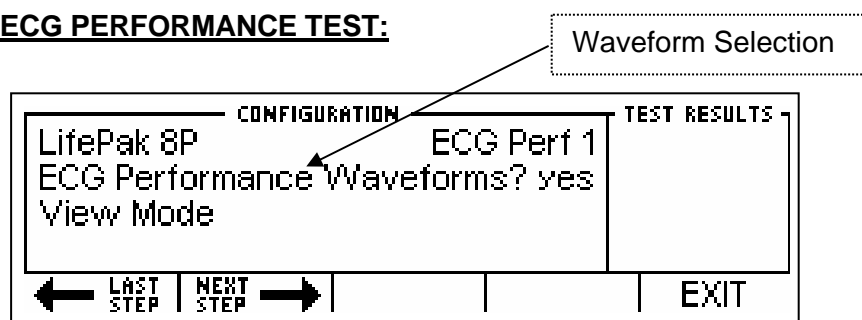DEFIBRILLATOR ECG PERFORMANCE TEST:


NOTE: The individual selected waveforms are not displayed in the VIEW MODE.

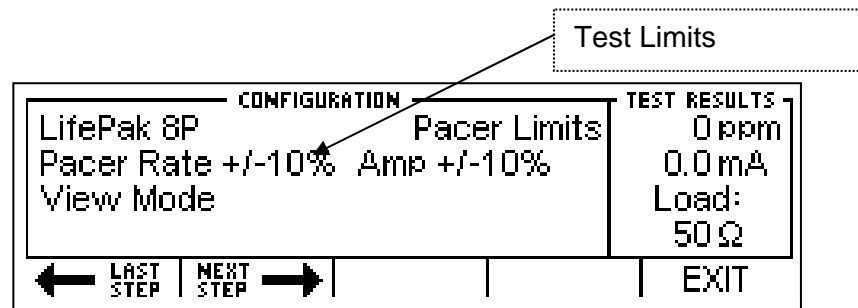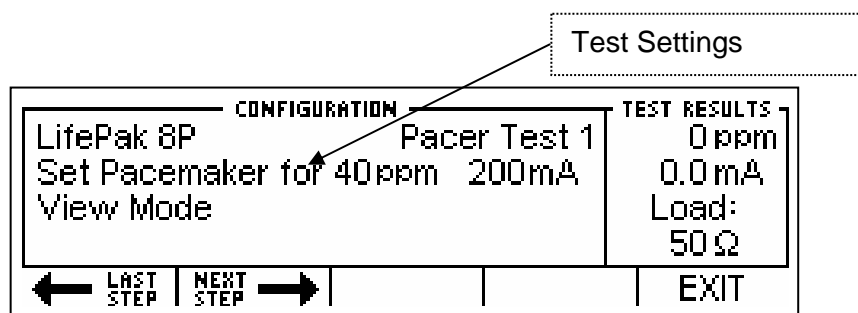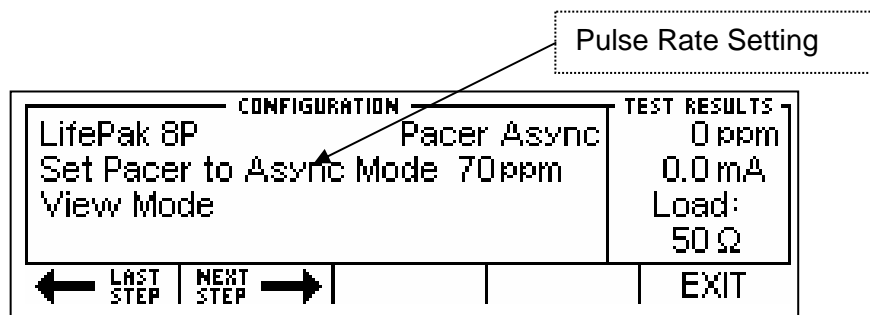PACEMAKER PULSE AND AMPLITUDE TESTS:**PACEMAKER ASYNCHRONOUS MODE TEST:**

PACEMAKER DEMAND MODE TESTS:

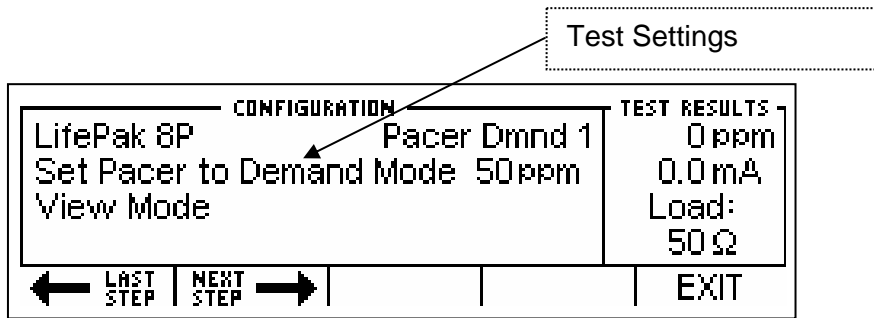

PACEMAKER REFRACTORY TEST:

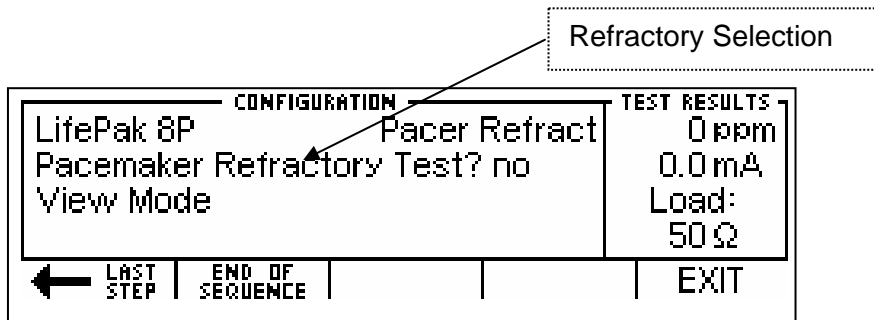

RUN MODE


The RUN MODE allows the user to run the test configuration. The screens that are displayed in the RUN MODE are determined by the Auto Sequence selected on the AUTO SEQUENCE SCREEN and its configuration as defined with the PC program.

Running an Auto Sequence will provide a consistent, guided procedure for testing equipment. This is a semi-automated process that will provide immediate feedback to the user if the DUT passes or fails individual tests. A programmable timer is provided to automatically progress through the test when a given test passes. This timer is set in the Auto Sequence Timer parameter in the SYSTEM SETUP SCREEN.

NOTE: If any particular test option is disabled using the PC Program, it will not be shown in the RUN MODE.

NOTE: Some tests, like Performance Waveforms, do not have quantitative analyses and therefore require the user to manually progress through the test.

The following sample screen shows the common elements present during the RUN MODE:

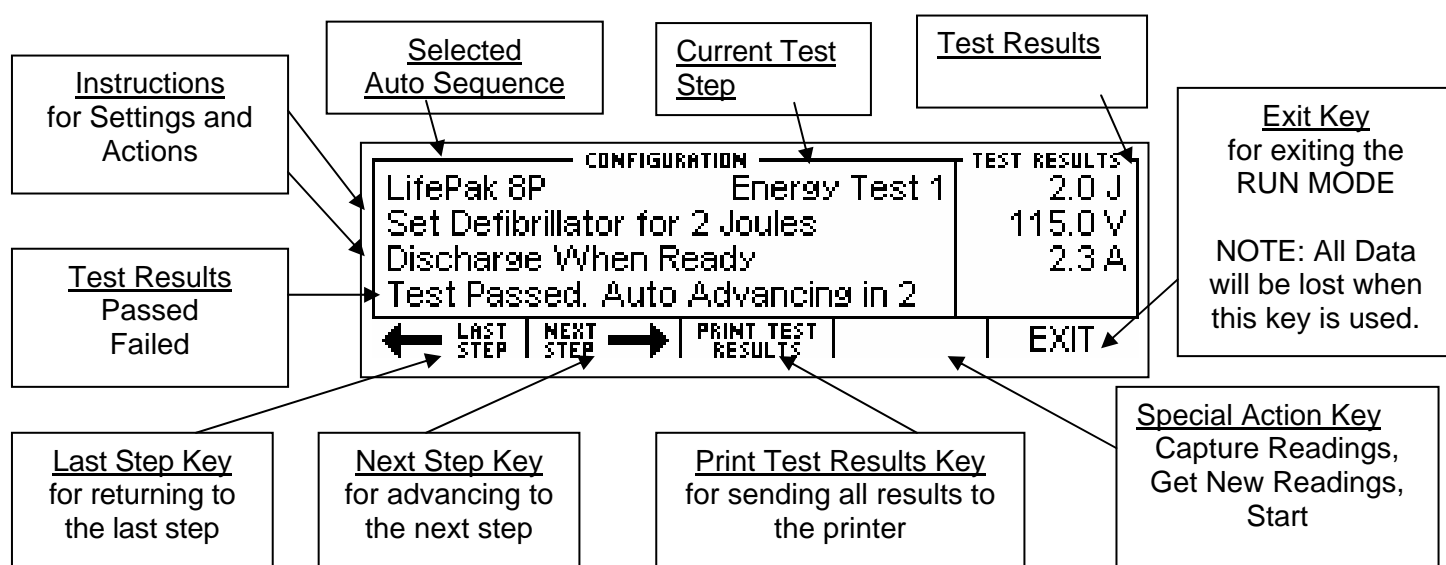

The following screens may be shown in the RUN MODE if all test options are selected:

DEFIBRILLATOR ENERGY TESTS

Test Setup and Action

CONFIGURATION		TEST RESULTS
LifePak 8P	Energy Test 1	0.0 J
Set Defibrillator for 2 Joules		0.0 V
Discharge When Ready		0.0 A
← LAST STEP	NEXT STEP →	PRINT TEST RESULTS
		EXIT

Test Passed

CONFIGURATION		TEST RESULTS
LifePak 8P	Energy Test 1	2.0 J
Set Defibrillator for 2 Joules		115.0 V
Discharge When Ready		2.3 A
Test Passed. Auto Advancing in 2		
← LAST STEP	NEXT STEP →	PRINT TEST RESULTS
		EXIT

Test Failed

CONFIGURATION		TEST RESULTS
LifePak 8P	Energy Test 1	5.1 J
Set Defibrillator for 2 Joules		183.0 V
Discharge When Ready		3.7 A
Test Failed. Retry if desired		
← LAST STEP	NEXT STEP →	PRINT TEST RESULTS
		EXIT

DEFIBRILLATOR MAXIMUM ENERGY TESTS:

Test Setup and Action

CONFIGURATION		TEST RESULTS
LifePak 8P	MaxE Chg Time	0.0 J
Set Defibrillator for 360 Joules		0.0 V
Press Start Timer When Ready		0.0 A
		0.0 S
← LAST STEP	NEXT STEP →	PRINT TEST RESULTS
		START CHARGE TIMER
		EXIT

Charge Timer Warning

CONFIGURATION		TEST RESULTS
LifePak 8P	Charge Timer Will Begin in	0.0 J
Set Defibri	4 Seconds	0.0 V
Press Star	Or Press Cancel to Exit	0.0 A
		0.0 S
		CANCEL

Charge Timer Running

CONFIGURATION		TEST RESULTS
LifePak 8P	Charge Timer Running	337.5 J
Set Defibri	4.5 Seconds	2470.0 V
Press Star	Defib When Charged	49.4 A
Test Failed		21.6 S
		CANCEL

Results

CONFIGURATION		TEST RESULTS
LifePak 8P	MaxE Chg Time	338.7 J
Set Defibrillator for 360 Joules		2477.5 V
Press Start Timer When Ready		49.6 A
Test Passed. Auto Advancing in 3		8.8 S
← LAST STEP	NEXT STEP →	PRINT TEST RESULTS
		START CHARGE TIMER
		EXIT

DEFIBRILLATOR CARDOVERSION TESTS:

Test Setup and Action

CONFIGURATION		TEST RESULTS
LifePak 8P	Crdvrsn Test 1	0.0 J
Set Defibrillator for 100 Joules		0.0 V
Discharge Sync Mode When Ready		0.0 A
		0 mS
← LAST STEP	NEXT STEP →	PRINT TEST RESULTS
		EXIT

Test Passed


CONFIGURATION		TEST RESULTS
LifePak 8P	Crdvrsn Test 1	98.1 J
Set Defibrillator for 100 Joules		1340.0 V
Discharge Sync Mode When Ready		26.8 A
Test Passed. Auto Advancing in 3		26 mS
← LAST STEP	NEXT STEP →	PRINT TEST RESULTS
		EXIT

DEFIBRILLATOR ECG PERFORMANCE TEST:

Waveform



CONFIGURATION		TEST RESULTS
LifePak 8P	ECG Perf 2	Check ECG
ECG: Performance Waveforms		On Defib
Triangle Wave 2 Hz		Then Press
Lead I 0.70mV Lead II 1.0mV		Next Step
← LAST STEP	NEXT STEP →	PRINT TEST RESULTS
		EXIT

NOTE: Some tests, like Performance Waveforms, do not have quantitative analyses and therefore require the user to manually progress through the test.

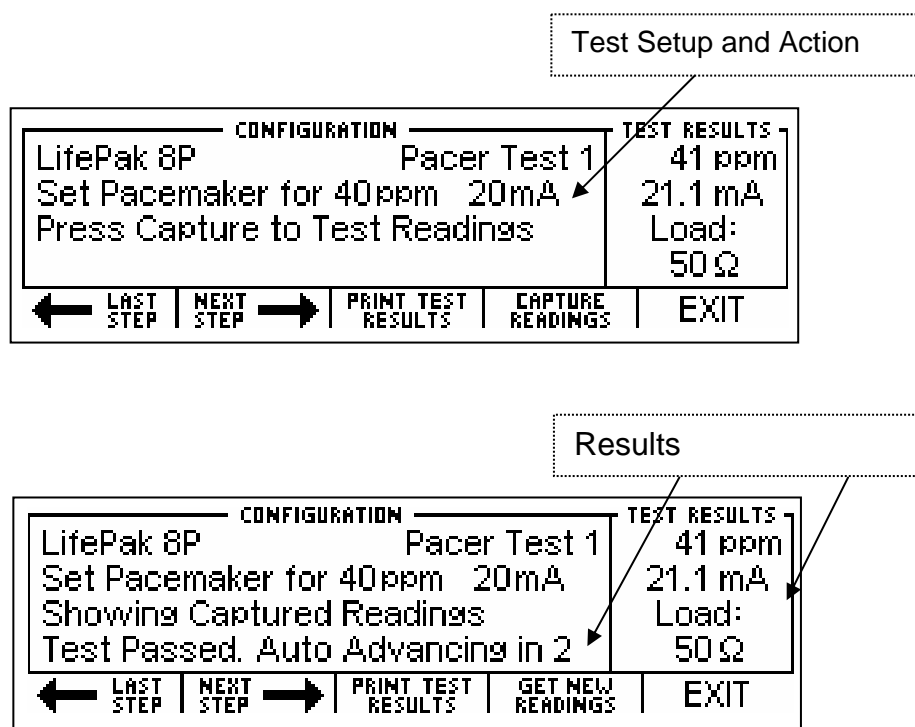PACEMAKER PULSE AND AMPLITUDE TESTS:

NOTE: If the test fails or new readings are desired, the Get New Readings Key can be used to replace the current readings. The current readings will be lost, even if they are from a test that passed.

PACEMAKER ASYNCHRONOUS MODE TEST

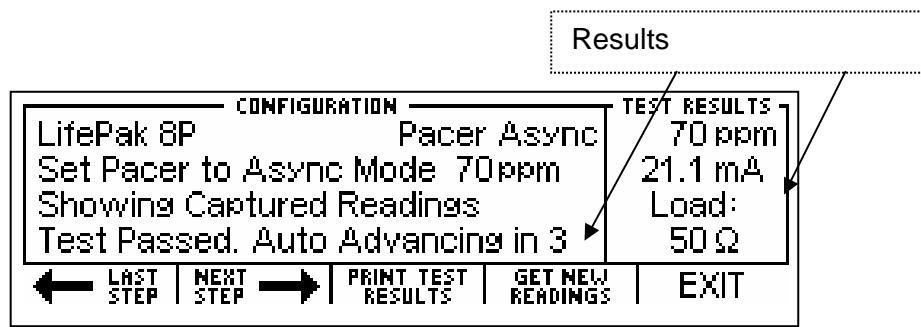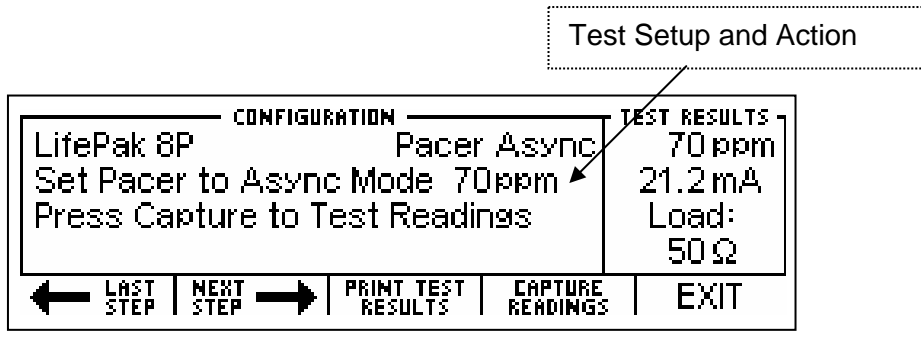

NOTE: If the test fails or new readings are desired, the Get New Readings Key can be used to replace the current readings. The current readings will be lost, even if they are from a test that passed.

PACEMAKER DEMAND MODE TESTS:

Test Setup and Action

CONFIGURATION		TEST RESULTS
LifePak 8P	Pacer Dmnd 1	51 ppm
Set Pacer to Demand Mode	50ppm	10.3 mA
Press Start for Sensitivity test		Load:
Sens.Pads: 0.00 mV	ECG: 0.00 mV	50 Ω
← LAST STEP	NEXT STEP →	PRINT TEST RESULTS
		START
		EXIT

Sensitivity Test Running

CONFIGURATION		TEST RESULTS
LifePak 8P	Sensitivity Test Running	51 ppm
Set Pacer	<div style="border: 1px solid black; width: 100px; height: 15px; margin: 2px 0;"></div>	10.5 mA
Press Start	Please Wait	Load:
Sens.Pads	Or Press Cancel to Exit	50 Ω
		CANCEL

Results

CONFIGURATION		TEST RESULTS
LifePak 8P	Pacer Dmnd 1	51 ppm
Set Pacer to Demand Mode	50ppm	10.5 mA
Showing Captured Readings		Load:
Sens.Pads: 4.86 mV	ECG: 0.65 mV	50 Ω
← LAST STEP	NEXT STEP →	PRINT TEST RESULTS
		GET NEW READINGS
		EXIT

NOTE: If the test fails or new readings are desired, the Get New Readings Key can be used to replace the current readings. The current readings will be lost, even if they are from a test that passed.

PACEMAKER REFRACTORY TEST:

Test Setup and Action

CONFIGURATION		TEST RESULTS
LifePak 8P	Pacer Refract	51 ppm
Set Pacemaker to Demand Mode		10.5 mA
Press Start for Refractory test		Load:
PaceRP: 0 mS	SensRP: 0 mS	50 Ω
← LAST STEP	END OF SEQUENCE	PRINT TEST RESULTS
		START
		EXIT

Refractory Test Running

CONFIGURATION		TEST RESULTS
LifePak 8P	Refractory Test Running	51 ppm
Set Pacem		10.1 mA
Press Star	Please Wait	Load:
PaceRP:	Or Press Cancel to Exit	50 Ω
		CANCEL

Results

CONFIGURATION		TEST RESULTS
LifePak 8P	Pacer Refract	51 ppm
Set Pacemaker to Demand Mode		10.1 mA
Showing Captured Readings		Load:
PaceRP: 284 mS	SensRP: 290 mS	50 Ω
← LAST STEP	END OF SEQUENCE	PRINT TEST RESULTS
		GET NEW READINGS
		EXIT

NOTE: If the test fails or new readings are desired, the Get New Readings Key can be used to replace the current readings. The current readings will be lost, even if they are from a test that passed.

EXITING AUTO SEQUENCE TESTING MESSAGE

The “Exit Auto Sequence Test All Data Will be Lost!” message will display in the Auto Sequencing Mode when is pushed. If the data is needed, it should be printed prior to exiting.

LifePak 8P	<u>Exit AutoSequence Test</u>	TEST RESULTS
Set Pacem	All Data Will be Lost!	0 ppm
Press Star	Are You Sure?	0.0 mS
PaceRP:		0.0 mA
		0.0 mJ
		YES
		NO


This page intentionally left blank.

PROGRAMMING AUTO SEQUENCES

Auto Sequences are programmed with an easy to use PC interface. This section shows how to use the Auto Sequence configuration software.

SPLASH SCREEN

The Splash Screen identifies the version of the program. This screen will be displayed for 5 seconds, or until the user presses a key or clicks the screen with the mouse.

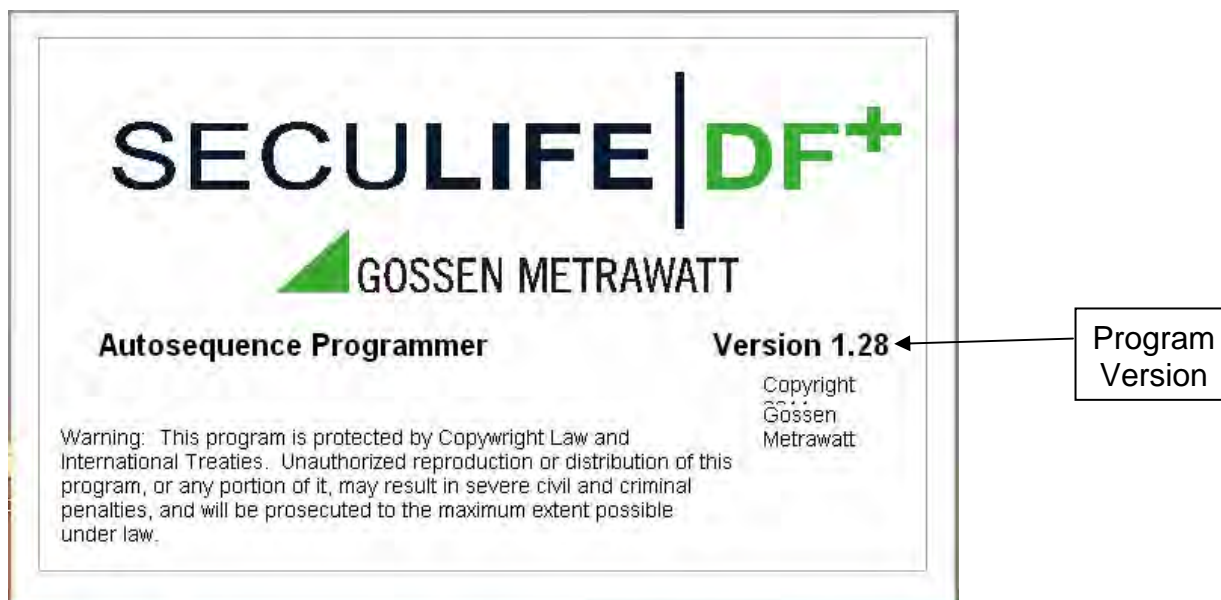

OVERVIEW

The following is a general overview of the PC Interface used for Programming Auto Sequences. Each part of this screen is described in full detail later in this section.

Program Menu Bar
The top of the window contains a menu bar with 'File' and 'Help' options.

File Control
This section is utilized to load/save configuration files on the PC as well as read/write the auto configuration in the SECULIFE DF+.

ECG Sequence Programming
Use this section to easily configure each step of the ECG Auto Sequence.

Sequence Selection
Use this list to select which sequence to view /edit.

Status Message
A small area at the bottom left of the main window for displaying status information.

Com Port being used
A dropdown menu at the bottom left of the main window to select the serial port.

AutoSequence Filename
A dropdown menu at the top center for selecting the current sequence file.

ECG Performance Test Sequence
A detailed configuration panel on the right side for setting parameters for each step of the ECG test, including output groups, waveforms, and amplitudes.

Energy Level Test (0 J to End)
A table for configuring energy levels for each step of a test.


Step	Energy Level (Joules)
Step 1	10
Step 2	25
Step 3	50
Step 4	100
Step 5	200
Step 6	300
Step 7	400
Step 8	450
Step 9	0
Step 10	0
Step 11	0
Step 12	0
Step 13	0
Step 14	0
Step 15	0
Step 16	0
Step 17	0
Step 18	0
Step 19	0
Step 20	0

Task Progress Indicator
A progress bar at the bottom center of the main window.

Current Time
A digital clock display at the bottom right of the main window.

Today's Date
A digital date display at the bottom right of the main window.

Sequence Configuration
Use this section to configure each Auto Sequence test.

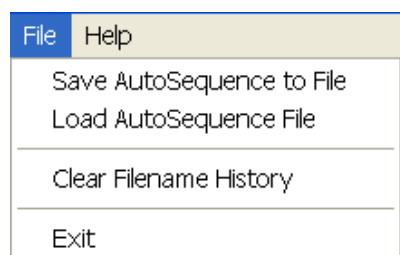
PROGRAM MENU

The program menu contains shortcuts to file operations as well as program version information.

From the File Menu, you can Save or Load Auto Sequences as well as Clear the History of files that were used. You can also Exit the program from this menu.




The Help Menu provides access to program version information, shown below:

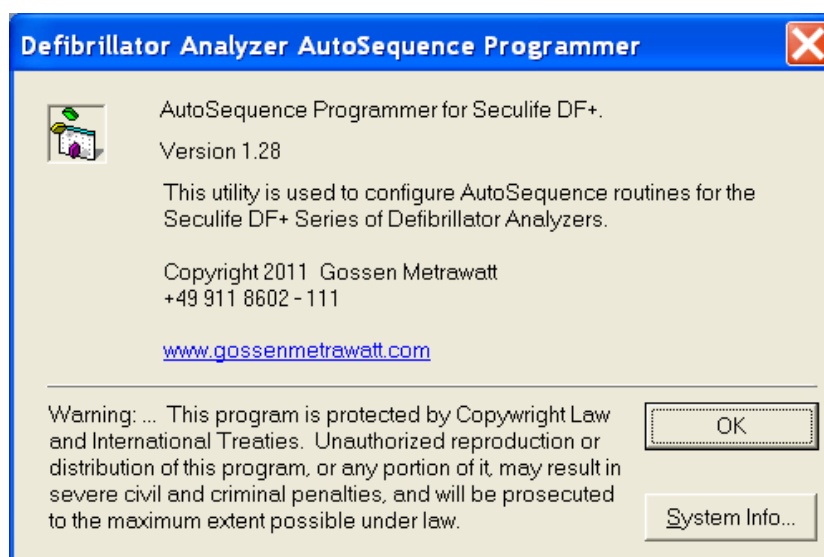

FILE CONTROL

The file control section allows the user to Load and Save Auto Sequence files, greatly expanding the number of pre-programmed sequences from 50 to virtually unlimited. The user also uses the File Control section to Load and Store Auto Sequences on the SECULIFE DF+.

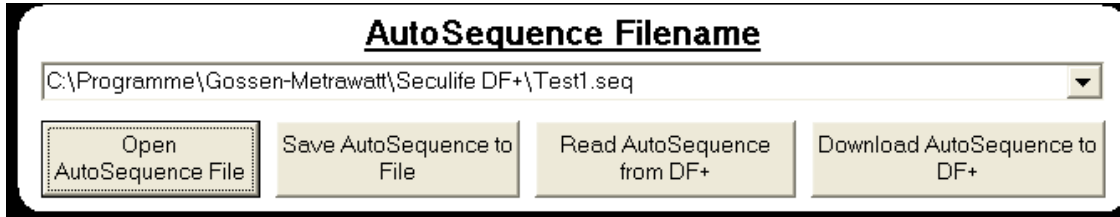

Dropdown List – This list shows the history of files that have recently been used. This provides quick access for switching between common Auto Sequence files.


Open Auto Sequence File – This button brings up the standard Windows Open File dialog box. It is used to load an existing configuration file.

Save Auto Sequence to File – This button brings up the standard Windows Save File dialog box. It is used to save the current configuration to a file for future reference.

Read Auto Sequence from SECULIFE DF+ – This button is used to load the configuration currently stored in the SECULIFE DF+.

Download Auto Sequence to SECULIFE DF+ – This button is used to send the configured Auto Sequence to the SECULIFE DF+, where it is stored in non-volatile flash memory.


SEQUENCE SELECTION

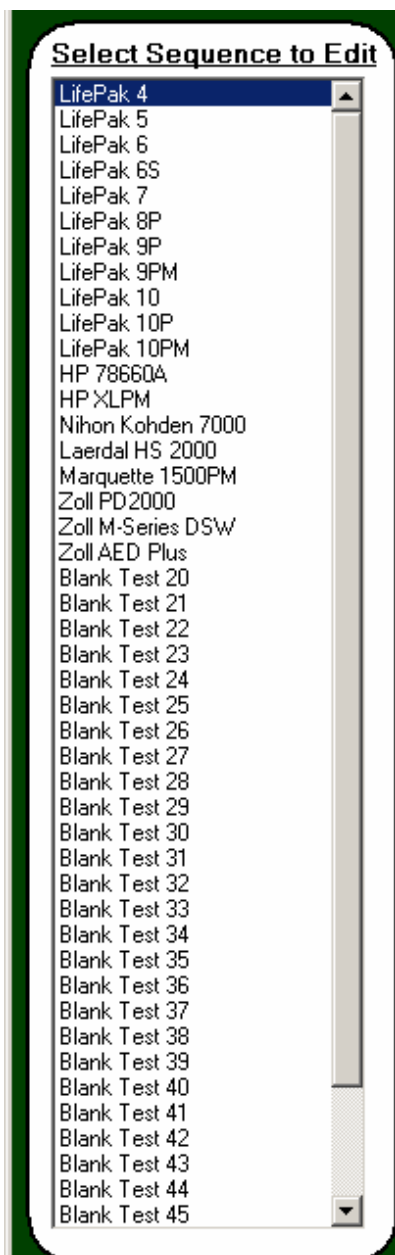

This section shows a list of all of the names of the Auto Sequences. It is used to select an individual sequence for configuration. Once selected, the configuration window will change to display the settings for the selected sequence.

SEQUENCE CONFIGURATION

The sequence configuration window displays all of the configuration settings for each Auto Sequence. This sample screen shows a defib test configuration.

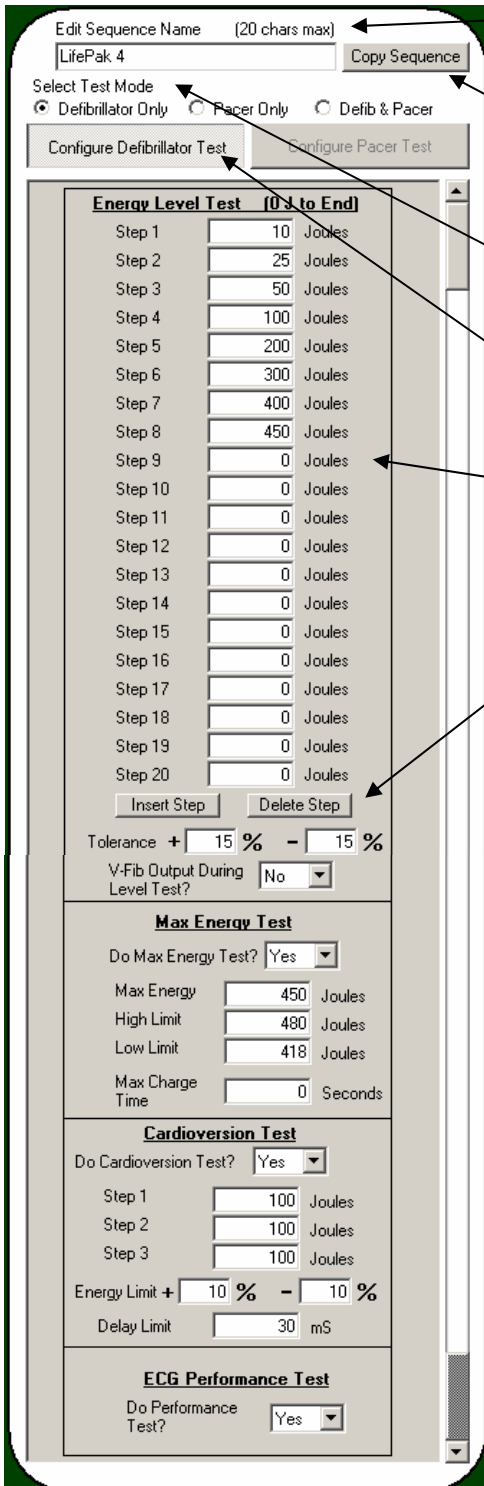

Sequence Name – This name can be any string of up to 20 standard ASCII characters. NOTE: Not all ASCII characters are valid and will be ignored.

Copy Sequence Button – This button opens the Copy Sequence Screen that allows the user to quickly configure similar test sequences.

Test Mode Selections – These selections allow each test to be configured as a Defibrillator Only, a Pacer Only or a Defib & Pacer test.

Configure Test Buttons – These buttons are used to alternate between defib and pacer test configuration windows.

Defibrillator Test Details – Each of the potential tests and test details for the Defibrillator are displayed for configuration. For ease of programming, individual steps can be deleted or added and individual tests can be included or not included.

Insert and Delete Steps Buttons – These buttons will open the Insert Steps Screen or the Delete Steps Screen.

Edit Sequence Name (20 chars max)
 LifePak 9PM Copy Sequence

Select Test Mode
 Defibrillator Only Pacer Only Defib & Pacer

Configure Defibrillator Test Configure Pacer Test

Pulse Mode Tests (0 ppm to End)

Step 1	60	ppm	55	mA	700	Ohms
Step 2	150	ppm	55	mA	700	Ohms
Step 3	170	ppm	55	mA	700	Ohms
Step 4	160	ppm	55	mA	700	Ohms
Step 5	140	ppm	55	mA	700	Ohms
Step 6	130	ppm	55	mA	700	Ohms
Step 7	120	ppm	55	mA	700	Ohms
Step 8	110	ppm	55	mA	700	Ohms
Step 9	100	ppm	55	mA	700	Ohms
Step 10	90	ppm	55	mA	700	Ohms
Step 11	80	ppm	55	mA	700	Ohms
Step 12	70	ppm	55	mA	700	Ohms
Step 13	60	ppm	55	mA	700	Ohms
Step 14	50	ppm	55	mA	700	Ohms
Step 15	40	ppm	55	mA	700	Ohms
Step 16	60	ppm	200	mA	700	Ohms
Step 17	60	ppm	150	mA	700	Ohms
Step 18	60	ppm	100	mA	700	Ohms
Step 19	60	ppm	130	mA	700	Ohms
Step 20	0	ppm	0	mA	Defib	Ohms

Insert Step Delete Step

Rate Tol ± 10 % Amp Tol ± 10 %

Async Mode Test
 Do Async Mode Test? Yes
 Rate 60 ppm Load 100 Ohms

Demand Mode Tests (0 ppm to End)
 Do Demand Mode Test? Yes

	Rate (ppm)	Face Load (Ohms)	Output Waveform
Step 1	50	700	40 mS Square
Step 2	0	Defib	10 mS Square
Step 3	0	Defib	10 mS Square
Step 4	0	Defib	10 mS Square
Step 5	0	Defib	10 mS Square


Refractory Mode Test
 Do Refractory Mode Test? No

Pacer Test Details – Each of the potential tests and test details for the Pacer are displayed for configuration. For ease of programming, individual steps can be deleted or added and individual tests can be included or not included.

Insert and Delete Steps Buttons – These buttons will open the Insert Steps Screen or the Delete Steps Screen.

Copy Sequence Screen

This function allows the user to quickly configure similar Auto Sequences. Simply select the source and target test sequences, press OK, and the target sequence will be overwritten with the configuration from the source sequence configuration. The Cancel button will exit the window without modifying any configuration settings.

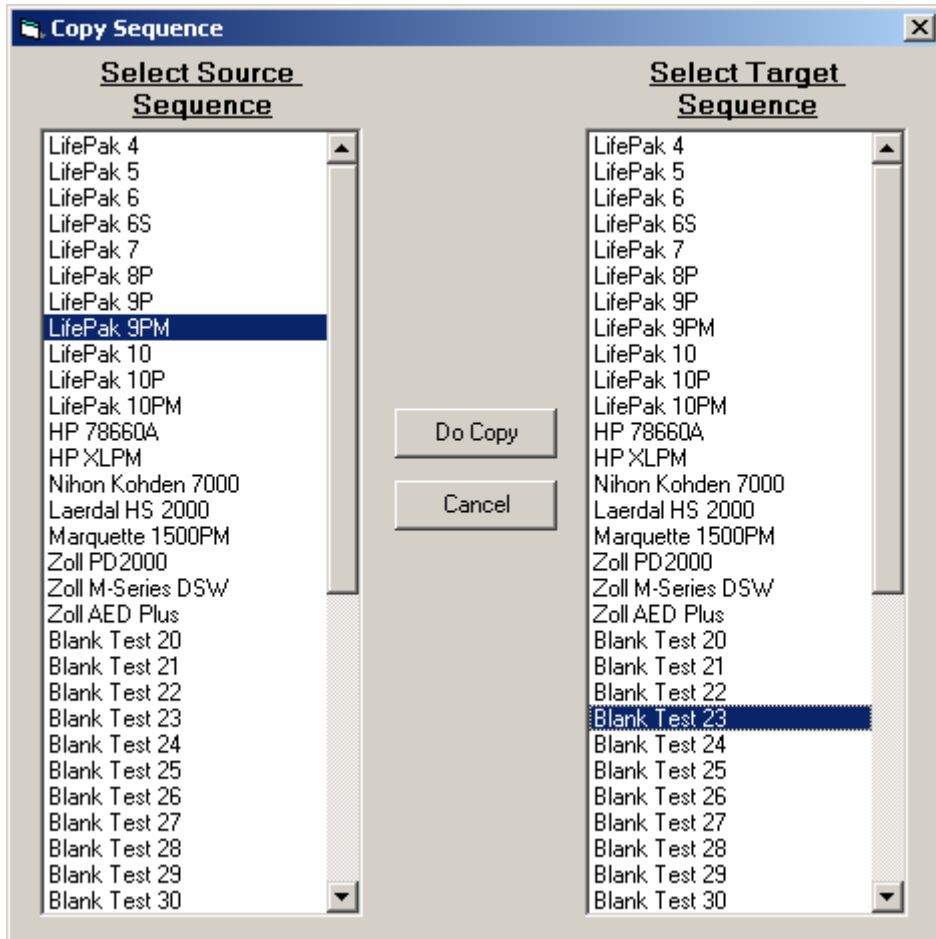

Insert Step and Deleting Step Screens

The insert and delete functions allow the user to quickly modify an existing test configuration. Deleting a step will move all of the tests following the deleted test up by one step and clear the final step. Inserting a step will shift all following steps down by one step and clear the selected step location.

Defibrillator Examples:

Step	Joules
Step 1	10
Step 2	25
Step 3	50
<input checked="" type="radio"/> Step 4	100
Step 5	200
Step 6	300
Step 7	400
Step 8	450
Step 9	0
Step 10	0
Step 11	0
Step 12	0
Step 13	0
Step 14	0
Step 15	0
Step 16	0
Step 17	0
Step 18	0
Step 19	0
Step 20	0

Pressing OK here would shift steps 4-19 down by one step and insert a blank step at step 4.

Step	Joules
Step 1	10
Step 2	25
Step 3	50
Step 4	100
<input checked="" type="radio"/> Step 5	200
Step 6	300
Step 7	400
Step 8	450
Step 9	0
Step 10	0
Step 11	0
Step 12	0
Step 13	0
Step 14	0
Step 15	0
Step 16	0
Step 17	0
Step 18	0
Step 19	0
Step 20	0

Pressing OK here would shift steps 6-20 up by one step and insert a blank step at step 20.

Pacer Examples:

Insert Autosequence Step

Select Where to Insert the Step

<input type="radio"/>	Step 1	40	ppm	200	mA	50	Ohms
<input type="radio"/>	Step 2	50	ppm	200	mA	50	Ohms
<input type="radio"/>	Step 3	0	ppm	200	mA	50	Ohms
<input checked="" type="radio"/>	Step 4	70	ppm	200	mA	50	Ohms
<input type="radio"/>	Step 5	80	ppm	200	mA	50	Ohms
<input type="radio"/>	Step 6	90	ppm	200	mA	50	Ohms
<input type="radio"/>	Step 7	90	ppm	180	mA	50	Ohms
<input type="radio"/>	Step 8	80	ppm	170	mA	50	Ohms
<input type="radio"/>	Step 9	70	ppm	160	mA	50	Ohms
<input type="radio"/>	Step 10	60	ppm	150	mA	50	Ohms
<input type="radio"/>	Step 11	50	ppm	140	mA	50	Ohms
<input type="radio"/>	Step 12	40	ppm	130	mA	50	Ohms
<input type="radio"/>	Step 13	30	ppm	120	mA	50	Ohms
<input type="radio"/>	Step 14	33	ppm	110	mA	50	Ohms
<input type="radio"/>	Step 15	35	ppm	100	mA	50	Ohms
<input type="radio"/>	Step 16	36	ppm	90	mA	50	Ohms
<input type="radio"/>	Step 17	37	ppm	80	mA	50	Ohms
<input type="radio"/>	Step 18	38	ppm	70	mA	50	Ohms
<input type="radio"/>	Step 19	39	ppm	60	mA	50	Ohms
<input type="radio"/>	Step 20	40	ppm	50	mA	50	Ohms

OK Cancel

Pressing OK here would shift steps 4-19 down by one step and insert a blank step at step 4.

Delete Autosequence Step

Select the Step to Delete

<input type="radio"/>	Step 1	40	ppm	200	mA	50	Ohms
<input type="radio"/>	Step 2	50	ppm	200	mA	50	Ohms
<input type="radio"/>	Step 3	0	ppm	200	mA	50	Ohms
<input type="radio"/>	Step 4	70	ppm	200	mA	50	Ohms
<input type="radio"/>	Step 5	80	ppm	200	mA	50	Ohms
<input type="radio"/>	Step 6	90	ppm	200	mA	50	Ohms
<input type="radio"/>	Step 7	90	ppm	180	mA	50	Ohms
<input checked="" type="radio"/>	Step 8	80	ppm	170	mA	50	Ohms
<input type="radio"/>	Step 9	70	ppm	160	mA	50	Ohms
<input type="radio"/>	Step 10	60	ppm	150	mA	50	Ohms
<input type="radio"/>	Step 11	50	ppm	140	mA	50	Ohms
<input type="radio"/>	Step 12	40	ppm	130	mA	50	Ohms
<input type="radio"/>	Step 13	30	ppm	120	mA	50	Ohms
<input type="radio"/>	Step 14	33	ppm	110	mA	50	Ohms
<input type="radio"/>	Step 15	35	ppm	100	mA	50	Ohms
<input type="radio"/>	Step 16	36	ppm	90	mA	50	Ohms
<input type="radio"/>	Step 17	37	ppm	80	mA	50	Ohms
<input type="radio"/>	Step 18	38	ppm	70	mA	50	Ohms
<input type="radio"/>	Step 19	39	ppm	60	mA	50	Ohms
<input type="radio"/>	Step 20	40	ppm	50	mA	50	Ohms

OK Cancel

Pressing OK here would shift steps 6-20 up by one step and insert a blank step at step 20.

ECG CONFIGURATION SECTION

**ECG Performance
Test Sequence**

Step 1

ECG Output Group
AED

ECG Output Waveform
Asystole

ECG Output Amplitude
Lead II = 1.0 mV

Step 2

ECG Output Group
Performance

ECG Output Waveform
Square 2 Hz

ECG Output Amplitude
Lead II = 1.0 mV

Step 3

ECG Output Group
Performance

ECG Output Waveform
Triangle 2 Hz

ECG Output Amplitude
Lead II = 1.0 mV

Step 4

ECG Output Group
Normal Sinus Rhythm

ECG Output Waveform
80 BPM

ECG Output Amplitude
Lead II = 1.0 mV

Step 5

ECG Output Group

2/25/2007 9:41 AM

This section configures the ECG Performance sequence when the ECG Performance Test option is set to YES for a Defibrillator Test.

The ECG sequence consists of up to 10 steps. Each step consists of a selected waveform group (Disabled, NSR, AED, Arrhythmia or Performance), output waveform and output amplitude.

There is only one ECG sequence for all 50 Auto Sequence tests.

To use less than 10 steps, set the ECG output group of the next step after the last to "Disabled."

This page intentionally left blank.

LIMITED WARRANTY

WARRANTY: GMC-I MESSTECHNIK GMBH WARRANTS ITS NEW PRODUCTS TO BE FREE FROM DEFECTS IN MATERIALS AND WORKMANSHIP UNDER THE SERVICE FOR WHICH THEY ARE INTENDED. THIS WARRANTY IS EFFECTIVE FOR TWELVE MONTHS FROM THE DATE OF SHIPMENT.

EXCLUSIONS: THIS WARRANTY IS **IN LIEU OF** ANY OTHER WARRANTY EXPRESSED OR IMPLIED, INCLUDING, BUT NOT LIMITED TO ANY IMPLIED WARRANTY OF **MERCHANTABILITY** OR FITNESS FOR A PARTICULAR PURPOSE.

GMC-I MESSTECHNIK GMBH IS NOT LIABLE FOR ANY INCIDENTAL OR CONSEQUENTIAL DAMAGES.

NO PERSON OTHER THAN AN OFFICER IS AUTHORIZED TO GIVE ANY OTHER WARRANTY OR ASSUME ANY LIABILITY.

REMEDIES: THE PURCHASER'S SOLE AND EXCLUSIVE REMEDY SHALL BE: (1) THE REPAIR OR REPLACEMENT OF DEFECTIVE PARTS OR PRODUCTS, WITHOUT CHARGE. (2) AT THE OPTION OF **GMC-I MESSTECHNIK GMBH**, THE REFUND OF THE PURCHASE PRICE.

SPECIFICATIONS

ENERGY OUTPUT MEASUREMENT GENERAL	
METHOD	Monophasic or Biphasic
LOAD RESISTANCE	50 ohm +/- 1%, non-inductive (<1 μ H)
DISPLAY RESOLUTION	0.1 Joules
MEASUREMENT TIME WINDOW	100 ms
ABSOLUTE MAX PEAK VOLTAGE	6000 Volts
PULSE WIDTH	100 ms
CARDIOVERSION	
DELAY	0 to 6000 ms
RESOLUTION	0.1 ms
ACCURACY	+/-2 ms

ENERGY OUTPUT MEASUREMENT HIGH RANGE	
VOLTAGE	\leq 5000 Volts
MAX CURRENT	100 Amps
MAX ENERGY	1000 Joules
ACCURACY	+/-2% of reading for >100 Joules +/-2 Joules for <100 Joules
TRIGGER LEVEL	100 Volts
PLAYBACK AMPLITUDE	1 mv / 1000 V Lead 1
TEST PULSE	125 Joules +/- 20%

ENERGY OUTPUT MEASUREMENT LOW RANGE	
VOLTAGE	<1000 Volts
MAX CURRENT	20 Amps
MAX ENERGY	50 Joules
ACCURACY	+/-2% of reading for >20 Joules +/- 0.4 Joules for <20 Joules
TRIGGER LEVEL	20 Volts
PLAYBACK AMPLITUDE	1 mV / 1000 V Lead 1
TEST PULSE	5 Joules +/-20%

ENERGY OUTPUT MEASUREMENT OTHER	
OSCILLOSCOPE OUTPUT	
HIGH MEASURE RANGE	1000:1 amplitude-attenuated
LOW MEASURE RANGE	200:1 amplitude-attenuated
WAVEFORM PLAYBACK	
OUTPUT	LEAD I & PLATES
SCREEN	200:1 Time Base Expansion
SYNC TIME MEASUREMENTS	
TIMING WINDOW	Starts at peak of each R-wave
TEST WAVEFORMS	All waveform simulations available
DELAY TIME ACCURACY	+/- 1 ms
CHARGE TIME MEASUREMENT	
From 0.1 to 99.9 sec	

ECG NSR	
RATE	30,40,45,60,80,90,100,120,140,160,180,200,220,240,260,280,300 BPM
ACCURACY	+/- 1%
AMPLITUDE	0.5,1.0,1.5,2.0 mV (Lead II)
ACCURACY	+/- 2% @ Lead II
HIGH LEVEL	200 times Amplitude
ACCURACY	+/- 5%
QRS DURATION	80ms

ECG PERFORMANCE	
SINE WAVE	0.1,0.2,0.5,5,10,40,50,60,100 Hz
SQUARE WAVE	0.125, 2.000 Hz
TRIANGLE WAVE	2.000, 2.500 Hz
PULSE WAVE	30,60,120 BPM; 60 ms width
AMPLITUDE	0.5,1.0,1.5,2.0 mV (Lead II)
RATE ACCURACY	+/- 1%
AMPLITUDE ACCURACY	+/- 2% @ Lead II

ECG GENERAL	
LEAD TO LEAD IMPEDANCE (RL, LL, RA, LA)	1000 ohm
LEAD TO LEAD IMPEDANCE (V1-V6)	1000 ohm

ECG ARRHYTHMIA SELECTIONS
Ventricular Fibrillation
Atrial Fibrillation
Second Degree A-V Block
Right Bundle Branch Block
Premature Atrial Contraction
PVC Early
PVC Standard
PVC R on T
Multifocal PVC
Bigeminy
Run of 5 PVCs
Ventricular Tachycardia

SHOCK ADVISORY ALGORITHM TEST ECG SIGNALS
Asystole
Coarse Ventricular Fibrillation
Fine Ventricular Fibrillation
Multifocal Ventricular Tachycardia @ 140 BPM
Multifocal Ventricular Tachycardia @ 160 BPM
Polyfocal Ventricular Tachycardia @ 140 BPM
Polyfocal Ventricular Tachycardia @ 160 BPM
SupraVentricular Tachycardia @ 90 BPM

TRANSCUTANEOUS PACEMAKER ANALYZER TEST LOAD	
RANGE	50,100,150,200,300,400,500,600,700, 800,900,1000,1100,1200,1300,1400, 1500,1600,1700,1800,1900,2000, 2100,2200,2300 ohms
ACCURACY	50 to 1300 ohm +/-1% 1400 to 2300 ohm +/-1.5%

TRANSCUTANEOUS PACEMAKER ANALYZER OSCILLOSCOPE OUTPUT	
0 – 15 V	10.24:1 amplitude attenuation
15 – 60 V	41:1 amplitude attenuation
> 60 V	164:1 amplitude attenuation
MAX OUTPUT	200 V

TRANSCUTANEOUS PACEMAKER ANALYZER PULSE MEASUREMENTS	
CURRENT	4 to 300 mA (100 ohm load)
ACCURACY	+/-5% or +/-0.5 mA (whichever is greater)
RATE	30 to 800 ppm
ACCURACY	+/-1% or 2 ppm (whichever is greater)
PULSE WIDTH	0.6 to 80 ms
ACCURACY	+/-1% or +/-0.3 ms (whichever is greater)
MAX VOLTAGE	200 V (Variable Load Input Jacks) 15 V (Fixed Load Input Jacks)
PACE LIMIT	
PACE LOAD (Ohms)	CURRENT (mA)
50	300
100	300
150	300
200	300
300	300
400	300
500	300
600	300
700	286
800	250
900	222
1000	200
1100	182
1200	167
1300	154
1400	143
1500	133
1600	125
1700	118
1800	111
1900	105
2000	100
2100	95
2200	91
2300	87


TRANSCUTANEOUS PACEMAKER ANALYZER DEMAND SENSITIVITY	
WAVEFORMS	
SELECTIONS	Square Triangle Haversine
WIDTH	10,25,40,100,200 ms
ECG OUTPUT	
AMPLITUDE – OUT	0 to 4 mV
RESOLUTION – OUT	40 μ V
ACCURACY – OUT	+/-2%
PACER INPUT (50 TO 400 OHMS)	
AMPLITUDE – OUT	0 to 10 mV / 50 Ohms
RESOLUTION – OUT	40 μ V
ACCURACY – OUT	+/-2%
RATE – IN	30 to 100 ppm
PACER INPUT (500 TO 2300 OHMS & OPEN)	
AMPLITUDE – OUT	0 to 100 mV
RESOLUTION – OUT	1mV
ACCURACY – OUT	+/-2%
RATE – IN	30 to 100 ppm
DEFIBRILLATOR PLATES	
AMPLITUDE – OUT	0 to 10 mV
RESOLUTION – OUT	0.1 mV
ACCURACY – OUT	+/-2%
RATE – IN	30 to 100 ppm

TRANSCUTANEOUS PACEMAKER ANALYZER 50/60 HZ INTERFERENCE TEST SIGNAL	
ECG OUTPUT	0,0.4,0.8,1.2,1.6,2.0,2.4,2.8, 3.2,3.6,4.0 mV
PACER INPUT 50 OHMS	0,1,2,3,4,5,6,7,8,9,10 mV
PACER INPUT 100 OHMS	0,2,4,6,8,10,12,14,16,18,20 mV
PACER INPUT 150 OHMS	0,3,6,9,12,15,18,21,24,27,30 mV
PACER INPUT 200 OHMS	0,4,8,12,16,20,24,28,32,26,40 mV
PACER INPUT 300 OHMS	0,6,12,18,24,30,36,42,48,54,60 mV
PACER INPUT 400 OHMS	0,8,16,24,32,40,48,56,64,72,80 mV
PACER INPUT \geq 500 OHMS	0,10,20,30,40,50,60,70,80,90,100 mV
DEFIBRILLATOR PLATES	0,1,2,3,4,5,6,7,8,9,10 mV

TRANSCUTANEOUS PACEMAKER ANALYZER REFRACTORY PERIOD	
PACING	20 to 500 ms
SENSING	20 to 500 ms
ACCURACY	+/-2 ms

DATA INPUT/OUTPUTS
Parallel Printer Port
RS-232C (for computer control)

PHYSICAL	
DISPLAY	LCD Graphical 240 X 64 Pixels, Backlit
ENCLOSURE	3.4 x 9.8 x 10.7 Inches (86.4 x 249 x 271.8 mm) Royalite R59 UL Flame Rating 94 V-0
WEIGHT	< 5 Lbs (< 2.3 Kg)
FACE PLATE	Lexan, Back printed
OPERATING RANGE	15 to 40 C
STORAGE RANGE	-20 to 65 C

ELECTRICAL	
POWER	Battery, 9 VDC (2 required)  Alkaline
BATTERY ELIMINATOR	BC20 - 21103 (120 VAC) (US Version) BC20 - 21101 (220 VAC) (Euro Version) 10V, 300 mA DC

Product Support

If required please contact:

GMC-I Messtechnik GmbH
Product Support Hotline
Phone +49 911 8602-0
Fax +49 911 8602-709
E-Mail support@gossenmetrawatt.com

Service Center

Repair and Replacement Parts Service Calibration Center * and Rental Instrument Service

When you need service, please contact:

GMC-I Service GmbH

Service Center

Thomas-Mann-Strasse 20
90471 Nürnberg • Germany
Phone +49 911 817718-0
Fax +49 911 817718-253
E-Mail service@gossenmetrawatt.com
www.gmci-service.com

This address is only valid in Germany.

Please contact our representatives or subsidiaries for service in other countries.

***DKD** Calibration Laboratory

for Electrical Quantities DKD – K – 19701
accredited per DIN EN ISO/IEC 17025:2005

Accredited measured quantities: direct voltage, direct current -values, DC -resistance, -
alternating voltage, -alternating current -values, AC active power, AC apparent power,
DC power, -capacitance, -frequency and temperature

Edited in Germany • Subject to change without notice • A pdf version is available on the Internet