



Federal Democratic Republic of Ethiopia

👉 EDICT OF GOVERNMENT 👈

In order to promote public education and public safety, equal justice for all, a better informed citizenry, the rule of law, world trade and world peace, this legal document is hereby made available on a noncommercial basis, as it is the right of all humans to know and speak the laws that govern them.

ET ISO 15301 (2012) (English): Animal
vegetables fats and oils --
Determination of sediment in crude fats
and oils -- Centrifuge method

ISO INSIDE



BLANK PAGE



**ETHIOPIAN
STANDARD**

ES ISO 15301:2012

First edition

**Animal and vegetable fats and oils-
Determination of sediment in crude fats and
oils---Centrifuge method**

(Identical with ISO 15301:2001)

ICS: 67.200.10

Published by Ethiopian Standards Agency
©ESA



Foreword

This Ethiopian Standard has been prepared under the direction of the Technical Committee for Animal and vegetables fats and oils (TC 23) and published by the Ethiopian Standards Agency (ESA).

The standard is identical with ISO 15301:2001, Animal and vegetable fats and oils -Determination of sediment in crude fats and oils - Centrifuge method, published by International Organization for Standardization (ISO).

For the purpose of this Ethiopian Standard, the adopted text shall be modified as follows.

- The phrase “International Standard” shall be read as “Ethiopian Standard”; and
- A full stop (.) shall substitute comma (,) as decimal marker.

Animal and vegetable fats and oils — Determination of sediment in crude fats and oils — Centrifuge method

1 Scope

This International Standard specifies a method for the determination in crude fats or oils of that sediment which can be separated by centrifugal force.

The method is applicable to crude oils and to oils with a sediment content of 0,03 ml per 100 g to 15 ml per 100 g, obtained by means of extraction and/or crushing.

The method is not applicable to fats which are not liquid at a temperature of 20 °C.

2 Normative reference

The following normative document contains provisions which, through reference in this text, constitute provisions of this International Standard. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. However, parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent edition of the normative document indicated below. For undated references, the latest edition of the normative document referred to applies. Members of ISO and IEC maintain registers of currently valid International Standards.

ISO 661:1989, *Animal and vegetable fats and oils — Preparation of test sample*

3 Term and definition

For the purposes of this International Standard, the following term and definition applies.

3.1

sediment

that part of the insoluble matter in a crude fat or oil which can be centrifugally separated and is the total amount of the unclear layer of components collected at the bottom of the measuring tube after centrifuging

NOTE The sediment contains, for example, phospholipids, impurities, dirt, etc. dispersed in a water-containing phase, and can be quantified according to this International Standard. Any white crystalline components deposited on top of and within the dark layer of insoluble materials are regarded as part of the sediment.

4 Principle

A homogenized test sample is subjected to centrifuging as specified. The amount of separated material, called sediment, is volumetrically measured in a calibrated centrifuge tube.

5 Apparatus

Usual laboratory apparatus and, in particular, the following.

5.1 Centrifuge tubes, of capacity 100 ml, pear- or cone-shaped, made from thoroughly annealed glass and fitted with a stopper (see Figures 1 and 2).

NOTE Reading the volume of the unclear layer may be more difficult in a cone-shaped tube than in a pear-shaped tube.

5.2 Buckets, for centrifuge tubes (5.1), resistant to fats and oils.

5.3 Centrifuge, suitable for the centrifuge tubes (5.1) placed in the buckets (5.2), capable of controlling the rotational frequency so as to give a radial acceleration at the narrow part of the tubes of 700 to 800 times the acceleration of free fall.

See annex A for the calculation of the rotational frequency of the centrifuge.

In rooms which are not air-conditioned, use a centrifuge capable of maintaining its temperature between 20 °C and 25 °C.

5.4 Balance, capable of weighing to the nearest 0,1 g.

6 Sampling

It is important that the laboratory receive a sample which is truly representative and has not been damaged or changed during transport or storage.

Sampling is not a part of the method specified in this International Standard. A recommended sampling method is given in ISO 5555 [1].

Store samples in glass or polyethylene terephthalate (PET) bottles.

7 Preparation of test sample

Prepare the test sample in accordance with ISO 661.

Bring the test sample, if necessary, to a temperature of between 20 °C and 25 °C.

Redisperse any sediment in the oil from the bottom of the sample bottle to ensure a sufficiently homogeneous and representative sample. Immediately proceed in accordance with clause 8.

8 Procedure

Weigh two centrifuge tubes (5.1) to the nearest 0,1 g. Transfer 100 ml of the prepared test sample (clause 7) to each of the centrifuge tubes. Weigh the tubes and place them in the buckets (5.2) in the centrifuge (5.3). Adjust the rotational frequency so as to give a radial acceleration at the narrow part of tubes of 700 to 800 times the acceleration of free fall. Centrifuge for $1 \text{ h} \pm 5 \text{ s}$.

Read sediment volumes up to and including 1,5 ml to the nearest 0,03 ml. Read sediment volumes greater than 1,5 ml to the nearest 0,5 ml.

When using a cone-shaped tube, it may be more difficult to read the volume of the unclear layer; read the sediment volumes as accurately as possible.

If in a pear-shaped tube the separation is not complete (clear layer in the neck of the narrow tube section of the tube), the sediment reading should be corrected for this volume.

Record the relative radial acceleration or the swing diameter and the rotational frequency of the centrifuge.

Record the temperature before and after centrifuging.

9 Expression of results

Calculate the sediment content of the test sample using the equation:

$$w = \frac{V \times 100}{(m_1 - m_2)}$$

where

w is the numerical value of the sediment content of the test sample, in millilitres per 100 g;

V is the numerical value of the sediment volume, in millilitres;

m_1 is the numerical value of the mass of the centrifuge tube with the test portion, in grams;

m_2 is the numerical value of the mass of the centrifuge tube, in grams.

Calculate the mean of the results for the two tubes and report the results to the nearest 1 ml per 100 g.

10 Precision

10.1 Interlaboratory test

Details of interlaboratory tests on the precision of the method are given in annex B. The values derived from these tests may not be applicable to concentration ranges and matrices other than those given.

10.2 Repeatability

The absolute difference between two independent single test results, obtained using the same method on identical test material in the same laboratory by the same operator using the same equipment within a short interval of time, will in not more than 5 % of cases exceed the repeatability limit r given in or derived from Table 1.

Table 1 — Repeatability limit (r) and reproducibility limit (R)

Sediment content ml per 100 g	r ml per 100 g	R ml per 100 g
< 1	0,1	0,7
1 to 3	0,2	1,0

10.3 Reproducibility

The absolute difference between two single test results, obtained using the same method on identical test material in different laboratories by different operators using different equipment, will in not more than 5 % of cases exceed the reproducibility limit R given in or derived from Table 1.

11 Test report

The test report shall specify:

- all information necessary for the complete identification of the sample;
- the sampling method used, if known;
- the test method used, with reference to this International Standard;
- the relative radial acceleration or the swing diameter and the rotational frequency;

- the temperature before and after centrifuging;
- all operating details not specified in this International Standard, or regarded as optional, together with details of any incidents which may have influenced the test result(s);
- the test result obtained, or the two test results obtained if the repeatability has been checked.

Dimensions in millimetres

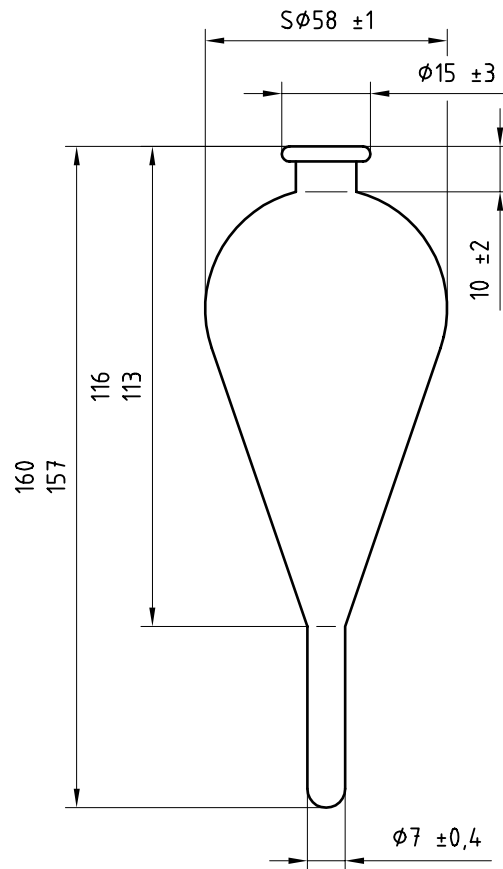


Figure 1 — Pear-shaped sediment tube

Dimensions in millimetres

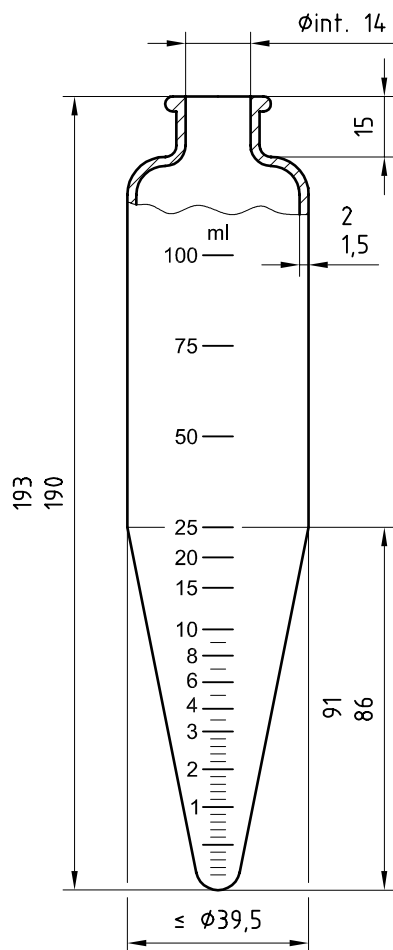


Figure 2 — Cone-shaped sediment tube

Annex A

(informative)

Calculation of the rotational frequency of a centrifuge

The rotational frequency of the centrifuge may be calculated by the equation:

$$n = 1\,337 \sqrt{\frac{a_r}{d}}$$

where

n is the numerical value of the rotational frequency, in min^{-1} ;

a_r is the relative radial acceleration (for example $a_r = 700$ or $a_r = 800$);

d is the numerical value of the diameter of swing, measured between the tips of opposite tubes when tubes are in a rotating position, in millimetres.

Annex B (informative)

Results of interlaboratory tests

B.1 Statistical results of interlaboratory tests

The precision of the method was established by two interlaboratory tests organized by the Netherlands Oils, Fats and Oilseeds Trade Association (NOFOTA) in cooperation with the Federation of Oils, Seeds and Fats Associations (FOSFA International) in 1996 and 1997/1998 and carried out in accordance with ISO 5725-2 [3]. In the first test 12 laboratories participated. Six (spiked) samples of crude sunflowerseed oil were investigated. In the second test 9 laboratories participated. Four (spiked) samples of crude sunflowerseed oil were investigated.

See Tables B.1 and B.2 for a summary of the statistical results of the tests.

Table B.1 — Statistical results of the interlaboratory test organized in 1996

Parameter	Sample					
	1	2	3	4	5	6
Number of laboratories retained after eliminating outliers	12	12	12	11	10	11
Mean sediment content, ml per 100 g	0,75	1,36	0,54	1,62	2,07	2,61
Repeatability standard deviation (s_r), ml per 100 g	0,04	0,06	0,04	0,06	0,03	0,07
Repeatability coefficient of variation, %	4,76	4,29	6,85	3,60	1,59	2,78
Repeatability limit (r) [$r = 2,8 \times s_r$], ml per 100 g	0,10	0,16	0,10	0,16	0,09	0,20
Reproducibility standard deviation (s_R), ml per 100 g	0,26	0,22	0,26	0,28	0,26	0,35
Reproducibility coefficient of variation, %	34,6	16,0	47,9	17,2	12,6	13,5
Reproducibility limit (R) [$R = 2,8 \times s_R$], ml per 100 g	0,72	0,61	0,72	0,78	0,73	0,99

Table B.2 — Statistical results of the interlaboratory test organized in 1997/1998

Parameter	Sample			
	1	2	3	4
Number of laboratories retained after eliminating outliers	7	8	8	7
Mean sediment content, ml per 100 g	0,07	1,28	1,20	2,39
Repeatability standard deviation (s_r), ml per 100 g	0,00	0,04	0,04	0,00
Repeatability coefficient of variation, %	0,00	2,77	2,95	0,00
Repeatability limit (r) [$r = 2,8 \times s_r$], ml per 100 g	0,00	0,10	0,10	0,00
Reproducibility standard deviation (s_R), ml per 100 g	0,07	0,12	0,08	0,35
Reproducibility coefficient of variation, %	97,8	9,1	7,0	14,8
Reproducibility limit (R) [$R = 2,8 \times s_R$], ml per 100 g	0,20	0,33	0,24	0,99

B.2 Comparison with the 96 h method

In the two interlaboratory tests, the centrifuge method was compared with the method which leaves the test sample to stand at a controlled temperature for 96 h.

Applying regression analysis to the results of both interlaboratory tests for the relation between the two methods, the following equation was established (with a correlation coefficient of 0,96):

$$w_2 = 2,5 w_1 - 0,5$$

where

w_1 is the numerical value of the sediment content obtained with the 96 h method, in millilitres per 100 ml;

w_2 is the numerical value of the sediment content obtained with the centrifuge method, in millilitres per 100 g.

This indicates that the centrifuge method may be considered as a good alternative to the 96 h method, where a rapid control method is required for levels of sediment exceeding 0,5 ml per 100 ml.

Bibliography

- [1] ISO 5555:1991, *Animal and vegetable fats and oils — Sampling*
- [2] ISO 5725-1:1994, *Accuracy (trueness and precision) of measurement methods and results — Part 1: General principles and definitions*
- [3] ISO 5725-2:1994, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*



Organization and Objectives

The Ethiopian Standards Agency (ESA) is the national standards body of Ethiopia established in 2010 based on regulation No. 193/2010. ESA is established due to the restructuring of Quality and Standards Authority of Ethiopia (QSAE) which was established in 1970.

ESA's objectives are:-

- ❖ Develop Ethiopian standards and establish a system that enable to check weather goods and services are in compliance with the required standards,
- ❖ Facilitate the country's technology transfer through the use of standards,
- ❖ Develop national standards for local products and services so as to make them competitive in the international market.

Ethiopian Standards

The Ethiopian Standards are developed by national technical committees which are composed of different stakeholders consisting of educational Institutions, research institutes, government organizations, certification, inspection, and testing organizations, regulatory bodies, consumer association etc. The requirements and/or recommendations contained in Ethiopian Standards are consensus based that reflects the interest of the TC representatives and also of comments received from the public and other sources. Ethiopian Standards are approved by the National Standardization Council and are kept under continuous review after publication and updated regularly to take account of latest scientific and technological changes.

Orders for all Ethiopian Standards, International Standard and ASTM standards, including electronic versions, should be addressed to the Documentation and Publication Team at the Head office and Branch (Liaisons) offices. A catalogue of Ethiopian Standards is also available freely and can be accessed in from our website.

ESA has the copyright of all its publications. No part of these publications may be reproduced in any form without the prior permission in writing of ESA.

International Involvement

ESA, representing Ethiopia, is a member of the International Organization for Standardization (ISO), and Codex Alimentarius Commission (CODEX). It also maintains close working relations with the international Electro-technical Commission (IEC) and American Society for Testing and Materials (ASTM). It is a founding member of the African Regional Organization for standardization (ARSO).

More Information?

Contact us at the following address.

The Head Office of ESA is at Addis Ababa.

☎ 011- 646 06 85, 011- 646 05 65

☎ 011-646 08 80

✉ 2310 Addis Ababa, Ethiopia

E-mail: info@ethiostandards.org,

Website: www.ethiostandards.org



Standard Mark